

OPERATOR'S
MANUAL


CADD  Prizm[®] VIP

Model 6100 and 6101

Ambulatory

Infusion

Pump

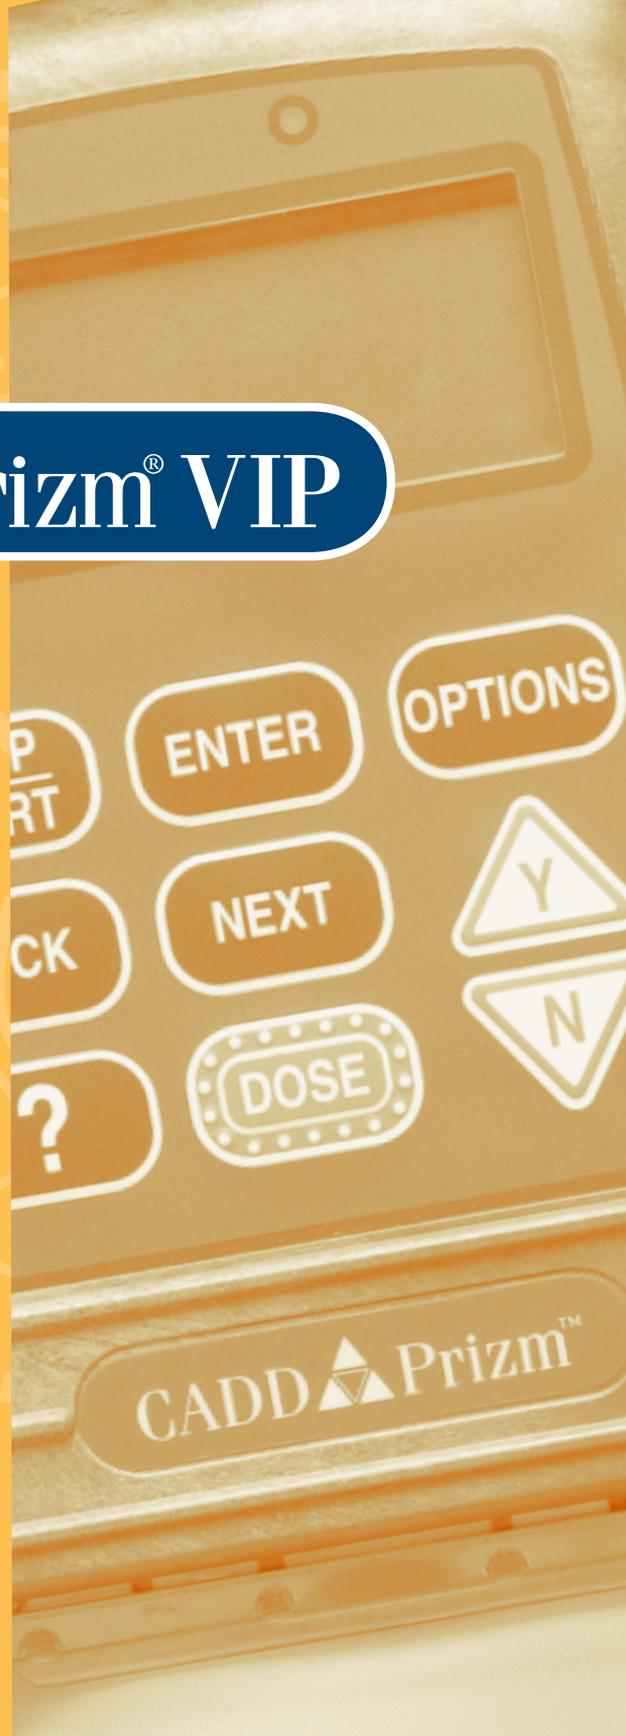

This manual concerns **only** the Deltec CADD-Prizm® VIP (Variable Infusion Profile) Model 6100 and Model 6101 ambulatory infusion pumps. The pump has the following delivery modes:

- PCA** **PCA 6210** (all revision letters)
- Continuous** **CONTIN 6220** (all revision letters)
- TPN** **TPN 6230** (all revision letters)
- Intermittent** **INTERMT 6240** (all revision letters)

This manual is intended for clinician use only. Do not permit patients to have access to this manual. The pump has three security levels designed to limit patient access. Do not disclose the pump’s security codes or any other information that would allow inappropriate access to programming and operating functions.

The issue date of this Operator’s Manual is included for the clinician’s information. In the event one year has elapsed between the issue date and product use, the clinician should contact SIMS Deltec, Inc. to see if a later revision of this manual is available.

Technical Assistance

If you have comments or questions concerning the operation of the CADD-Prizm® pump, please call the number given below. When calling, please specify the pump’s software module. This information is located in the pump’s start-up screen.

Our staff at Deltec is available to help clinicians twenty-four hours a day with the programming and operation of the CADD-Prizm® infusion system.

SIMS Deltec, Inc.
1265 Grey Fox Road
St. Paul, Minnesota 55112
1-800-426-2448

CADD, CADD-Prizm, Medication Cassette and Medication Cassette Reservoir design are SIMS trademarks.

DURACELL® is a registered trademark of DURACELL INC. EVEREADY® ENERGIZER® is a registered trademark of Union Carbide Corporation. ULTRALIFE® is a registered trademark of ULTRALIFE Batteries, Inc.

These products are covered by one or more of the following: U.S. Patent Nos. 4,559,038; 4,565,542; 4,650,469; 5,181,910; 5,338,157; 5,364,242; 5,485,408; 5,531,697; 5,531,698; 5,538,399; 5,540,561; 5,564,915; 5,567,136; 5,567,119; 5,695,473 for Model 6100 only; other patents pending.

Read this entire Operator's Manual before operating the CADD-Prizm® VIP ambulatory infusion pump.

Failure to properly follow warnings, cautions, and instructions could result in death or serious injury to the patient.

WARNINGS

- This Operator's Manual should be used by clinicians only. Do not permit patients to have access to this manual, as the information contained would allow the patient complete access to all programming and operating functions. Improper programming could result in death or serious injury to the patient.
- For those patients who are likely to be adversely affected by unintended operations and failures, including interrupted medication or fluid delivery from the device, close supervision and provision for immediate corrective action should be provided.
- If the pump is used to deliver life-sustaining medication, an additional pump must be available.
- The pump is not to be used for delivery of blood or cellular blood products.
- If the pump is dropped or hit, inspect the pump for damage. Do not use a pump that is damaged or is not functioning properly. Contact Customer Service to return a pump for service.
- Use of a syringe with the CADD® Administration Set may result in UNDER-DELIVERY of medication. Syringe function can be adversely affected by variations in plunger dimension and lubricity, which can result in greater force required to move the syringe plunger. A syringe plunger will lose lubrication as it ages and, as a result, the amount of under-delivery will increase which could on occasion, be significant. Therefore, the type of medication and delivery accuracy required must be considered when using a syringe with the CADD® pump.

Clinicians must regularly compare the volume remaining in the syringe to the pump's displayed values such as RES VOL and GIVEN in order to determine whether under-delivery of medication is occurring and if necessary, take appropriate action.

- System delivery inaccuracies may occur as a result of back pressure or fluid resistance, which depends upon drug viscosity, catheter size, and extension set tubing (for example, microbore tubing).

- Do not administer drugs to the epidural space or subarachnoid space unless the drug is indicated for those spaces.
- To prevent the infusion of drugs that are not indicated for epidural space or subarachnoid space infusion, DO NOT use administration sets that incorporate injection sites.
- If a Medication Cassette™ Reservoir, CADD® Extension Set or CADD® Administration Set is used for epidural space or subarachnoid space drug delivery, it is strongly recommended that it be clearly differentiated from those used for other routes of infusion, for example, by color coding, or other means of identification.
- When the Air Detector is not installed, or is installed but turned off, the pump will not detect air in the fluid path. It is recommended that you periodically inspect the fluid path and remove any air to prevent air embolism.
- You must use a CADD® Extension Set with Anti-Siphon Valve or a CADD® Administration Set with either an integral or an add on Anti-Siphon Valve to protect against unregulated gravity infusion that can result from an improperly attached cassette.
- When the Upstream Occlusion Sensor is turned Off, the pump will not detect occlusions upstream (between pump and fluid container). It is recommended that you periodically inspect the fluid path for kinks, a closed clamp, or other upstream obstructions. Upstream occlusions may result in under- or non-delivery of medications.
- Do not disclose to the patient the pump's security codes or any other information that would allow the patient complete access to all programming and operating functions.
- Do not use rechargeable NiCad or nickel metal hydride (NiMH) batteries. Do not use carbon zinc ("heavy duty") batteries. They do not provide sufficient power for the pump to operate properly.
- Always have new batteries available for replacement. If power is lost, non-delivery of drug will occur.
- There is no pump alarm to alert users that a battery has not been properly installed or has become dislodged. An improperly installed or dislodged battery could result in loss of power and non-delivery of drug.

- If the pump is dropped or hit, the battery door may become broken or damaged. Do not use the pump if the battery door is damaged because the battery will not be properly secured; this may result in loss of power or non-delivery of drug.
- When you enter a new Demand Dose Lockout time, any lockout time in effect will be cleared. A Demand Dose could be requested and delivered immediately upon starting the pump, resulting in over-delivery.
- When you enter a new Max Doses per Hour value, any lockout time in effect will be cleared. A Demand Dose could be requested and delivered immediately upon starting the pump, resulting in over-delivery.
- Exercise care when using the Clinician Bolus function. Since there are no limits on the frequency of delivering a bolus, and since the amount of the bolus can be set as high as 20 ml (or the mg or mcg equivalent), you should not permit the patient to become familiar with the procedure for giving a Clinician Bolus.
- To prevent the patient from accessing the Clinician Bolus function, do not let the patient know the Clinician Bolus code.
- Always close the fluid path tubing with the clamp before removing the cassette from the pump to prevent unregulated gravity infusion.
- Attach the cassette properly. An improperly attached or detached cassette could result in unregulated gravity infusion of medication from the fluid container or a reflux of blood.
- Do not prime the fluid path with the tubing connected to a patient as this could result in over-delivery of medication or air embolism.
- Ensure that the entire fluid path is free of all air bubbles before connecting to the patient to prevent air embolism.
- If Demand Doses are currently locked out, changing the Date and/or Time will cancel the lockout period. This will allow a Demand Dose to be requested and delivered as soon as you restart the pump, resulting in over-delivery.

CAUTIONS

- Do not operate the pump at temperatures below +2°C (36°F) or above 40°C (104°F).
- Do not store the pump at temperatures below -20°C (-4°F) or above 60°C (140°F). Do not store the pump with a Medication Cassette™ Reservoir or CADD® Administration Set attached.
- Do not expose the pump to humidity levels below 10% or above 90% relative humidity.
- Do not store the pump for prolonged periods with the battery installed. Battery leakage could damage the pump.
- If you are using a Medication Cassette™ Reservoir in which the medication is frozen, thaw at room temperature only. *Do not heat in a microwave oven* as this may damage the product and cause leakage.
- Do not immerse the pump in cleaning fluid or water. Do not allow solution to soak into the pump, accumulate on the keypad, or enter the battery compartment, Data In/Out jack, Power jack or Air Detector port area. Moisture build-up inside the pump may damage the pump.
- Do not clean the pump with acetone, other plastic solvents, or abrasive cleaners, as damage to the pump may occur.
- Do not expose the pump to therapeutic levels of ionizing radiation as permanent damage to the pump's electronic circuitry may occur. The best procedure to follow is to remove the pump from the patient during therapeutic radiation sessions. If the pump must remain in the vicinity during a therapy session, it should be shielded, and its ability to function properly should be confirmed following treatment.
- Do not expose the pump directly to ultrasound, as permanent damage to the pump's electronic circuitry may occur.
- Do not use the pump in the vicinity of magnetic resonance imaging (MRI) equipment as magnetic fields may adversely affect the operation of the pump. Remove the pump from the patient during MRI procedures and keep it at a safe distance from magnetic energy.
- Do not use the pump near ECG equipment as the pump may interfere with the operation of the equipment. Monitor ECG equipment carefully when using this pump.
- Do not sterilize the pump.

- Do not use the pump in the presence of flammable anesthetics or explosive gases.
- Use only Deltec accessories as using other brands may adversely affect the operation of the pump.
- Check appropriate medication stability for time and temperature to assure stability with actual pump delivery conditions.

Table of Contents

WARNINGS	iii
CAUTIONS	vi
Section 1: General Description and Basic Operations	1
Introduction	1
Indications	1
Epidural/Subarachnoid	1
Pump Diagram	3
Description of Keys, Display and Features	4
The Main Screen	8
Getting Help Using the (?) Key	9
Lock Levels	10
AutoLock	10
Security Codes	10
Customizing the Security Codes	10
Lock Level Table	11
Section 2: Pump Setup and Programming	13
Installing a battery	13
Watching Power-Up	15
Changing the Lock Level	16
PCA Delivery Method	
PCA Programming Screens	18
PCA Programming Example	23
PCA: Programming with Upper Limits, Adjusting Doses in Lock Level 1	29
PCA: Starting a Clinician Bolus	30
PCA: Starting a Demand Dose	32
PCA: Stopping a Demand Dose or Clinician Bolus	33

Continuous Delivery Mode	
Continuous Programming Screens	34
Continuous Programming Example	37
CONTIN: Programming with Upper Limits, Adjusting Rate in Lock Level 1	39
TPN Delivery Mode	
TPN Programming Screens	40
TPN Programming Example	44
TPN: Starting Daily Infusion	47
Intermittent Delivery Mode	
Intermittent Programming Screens	48
Intermittent Programming Example	52
INTERMT: Stopping the Pump During the Cycle	55
Section 3: Operating the Pump	57
Removing a Cassette	57
Attaching a Cassette	58
Priming the Tubing and Connecting to the Patient	61
Setting the Lock Level for the Patient	63
Starting the Pump	65
Stopping the Pump	65
Resetting the Reservoir Volume	66
Section 4: Options	67
Overview: Accessing Options	67
Immediate Taper-Down: TPN	68
Prime	69
Time Remaining: Intermittent	70
Extended History, Viewing: PCA	71
Change the Delivery Mode	73
AutoLock	74
Time	75
Date	76
Air Detector On/Off	77
Event Log, Viewing	78

Section 5: Biomed Toolbox	79
Overview: Accessing the Biomed Toolbox	79
Micrograms On/Off (PCA Only)	80
Concentration Customization (PCA Only)	80
Extended History On/Off (PCA Only)	82
Max Doses Per Hour On/Off (PCA Only)	82
PM (Preventive Maintenance) Reminder	83
Custom Lock Level Code	83
Date Format	84
Power Source Status Display	85
Upstream Sensor On/Off (Model 6101 only)	85
Air Detector Requirement	86
Section 6: Reference & Troubleshooting	87
Troubleshooting	87
Alarms and Messages, Alphabetical List	89
Cleaning the Pump and Accessories	98
Exposure to Radiation or Magnetic Resonance Imaging (MRI)	100
PCA Delivery Mode: Continuous Rate Scroll Ranges	101
PCA Delivery Mode: Demand Dose, Clinician Bolus Scroll Ranges, Milliliters	101
PCA Delivery Mode: Demand Dose, Clinician Bolus Scroll Ranges, Milligrams	102
PCA Delivery Mode: Demand Dose, Clinician Bolus Scroll Ranges, Micrograms	103
Military Time Conversion Chart	104
Specifications (Nominal)	105
Printed Reports	109
Index	110
Limited Warranty	114

Section 1: General Description and Basic Operations

Introduction

The Deltec CADD-Prizm® ambulatory infusion pump provides measured drug therapy to patients in hospital or outpatient settings. Therapy should always be overseen by a physician or a certified, licensed healthcare professional. As appropriate, the patient should be instructed in using the pump.

Indications

The CADD-Prizm® pump is indicated for intravenous, intra-arterial, subcutaneous, intraperitoneal, epidural space, or subarachnoid space infusion.

PCA (Patient-Controlled Analgesia) delivery is used for therapies that require a continuous rate of infusion, patient-controlled demand doses, or both, such as patient-controlled analgesia.

Continuous delivery allows the infusion of drug at a constant, programmed rate.

TPN (Total Parenteral Nutrition) delivery allows the infusion of nutritional solutions or other fluids, with optional tapering at the beginning and end of infusion.

Intermittent delivery allows the infusion of a specific volume of drug at a regular, programmed interval.

Epidural/Subarachnoid Administration

The selected drug must be used in accordance with the indications included in the package insert accompanying the drug. Administration of any drug by this pump is limited by any warnings, precautions, or contraindications in the drug labeling.

Analgesics

Administration of analgesics to the epidural space is limited to use with indwelling catheters specifically indicated for either short- or long-term drug delivery.

Administration of analgesics to the subarachnoid space is limited to use with indwelling catheters specifically indicated for short-term drug delivery.

Anesthetics

Administration of anesthetics to the epidural space is limited to use with indwelling catheters specifically indicated for short-term drug delivery.


WARNING:

- Do not administer drugs to the epidural space or subarachnoid space unless the drug is indicated for administration to those spaces. Drugs not intended for epidural or subarachnoid space infusion could result in death or serious injury to the patient.
 - To prevent the infusion of drugs that are not indicated for epidural space or subarachnoid space infusion, DO NOT use administration sets that incorporate injection sites. The inadvertent use of injection sites for infusion of such drugs may cause death or serious injury to the patient.
 - If a Medication Cassette™ Reservoir, CADD® Extension Set or CADD® Administration Set is used for epidural space or subarachnoid space drug delivery, it is strongly recommended that it be clearly differentiated from those used for other routes of infusion, for example, by color coding, or other means of identification. Drugs not intended for epidural or subarachnoid space infusion could result in death or serious injury to the patient.
-
-

Pump Diagram



Front View

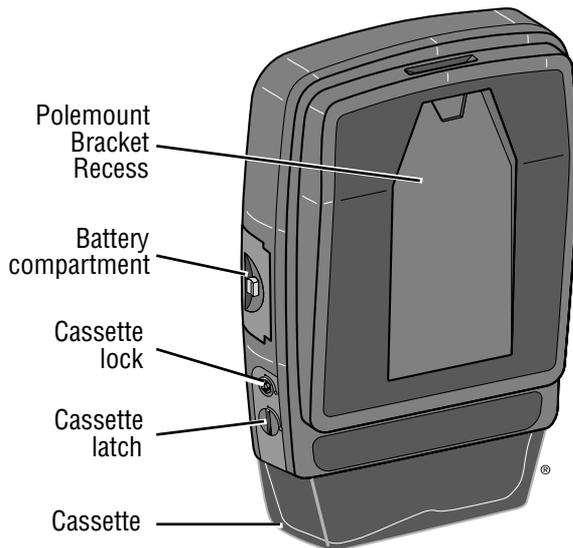

Rear View

Description of Keys, Display and Features

Indicator Lights

Green: The green light blinks approximately every 3 seconds when the pump is running and delivering fluid as programmed.

Amber: The amber light flashes when the pump is stopped or an alarm condition exists. It stays on continuously when the pump is inoperable. The display briefly describes the condition.

If both lights blink, delivery is still occurring but a condition exists of which you should be aware (for example, a low battery). Look at the display for a brief description of the condition.

Display with backlighting

The liquid crystal display (LCD) shows programming information and messages. Backlighting helps keep the display visible in low light.

After a period of no key presses, backlighting turns off and the display blanks to save battery power (except during an alarm or when an external power source is in use). Press any key to turn the display back on.

NOTE: If you press , the display will reappear with a message asking if you wish to start or stop the pump; press  or . Do not use  to turn the display back on; this may deliver an inadvertent dose.

Keypad

The keys on the keypad are described below. A key beeps when pressed if it is operable in the current lock level.



starts and stops pump delivery.



is used to view or change the pump's current lock level. Lock levels are used to limit patient access to certain programming and operating functions. (See Lock Levels, this section.) This key is also used to access the Clinician Bolus in the PCA delivery mode.



is the "Help" key. It is used to display help for a screen or an alarm message. (See Getting Help, this section.)



is used to enter, or save, a new value in the pump's memory when programming new pump settings. It is also used to select an item from the Options Menu (Section 4) or Biomed Toolbox Menu (Section 5).

NEXT

is used to move from one programming screen to the next without changing the setting or value displayed. It is also used to return from the Biomed Toolbox Menu to the Options Menu, or from the Options Menu to the main screen. (See Sections 4 and 5.)

DOSE

is used only in the PCA delivery mode. It allows the patient to deliver a programmed amount of medication upon request.

OPTIONS

is used to access the Options Menu, which contains such features as time, date, and the Event Log. (See Section 4, Options.)

Y

allows you to answer “yes” to a question on the pump’s display, “scroll up” or increase a value (for example, a dose amount), or scroll through items on a menu.

N

allows you to answer “no” to a question on the pump’s display, “scroll down” or decrease a value, scroll through items on a menu, or cancel printing.

Power jack

You may plug a CADD® External Power Source (EPS) System Power Pack or an AC Adapter into the Power jack as an alternate source of power.

Data In/Out jack

The Data In/Out jack is used for attaching the following accessories:

- **Interface Cable** for printing reports
- **Remote Dose Cord** for remote operation of the dose key
- **Modem cable** for communications

For more information on the Remote Dose Cord, printing or communications, see the instructions for use provided with those products.

Air Detector Port Cover

This encloses the Air Detector port when the Air Detector is not attached.

Air Detector accessory (optional)

The Air Detector attaches to the pump in the area shown in the diagram. If air is detected in the part of the tubing that passes through the Air Detector, an alarm sounds and delivery stops. (See Section 6 for Air Detector specifications.) The pump may be customized to require an Air Detector. (See Section 5, Biomed Toolbox.) If an Air Detector is attached but not required, it may be turned off.

WARNING: When the Air Detector is not installed, or is installed but turned off, the pump will not detect air in the fluid path. It is recommended that you periodically inspect the fluid path and remove any air to prevent air embolism. Air embolism could result in death or serious injury to the patient.

Cassette

The cassette is the portion of the Medication Cassette™ Reservoir or CADD® Administration Set that attaches to the bottom of the pump. The following single use products are compatible with the CADD-Prizm® pump:

- Medication Cassette™ Reservoir (50 or 100 ml), used with the CADD® Extension Set with Anti-Siphon Valve
 - CADD® Administration Set with integral or add on anti-siphon valve, for rates up to 125 ml/hr
 - CADD-Prizm® High Volume Administration Set, for rates up to 350 ml/hr (not for use in PCA mode)
-
-

WARNING: You must use a CADD® Extension Set with Anti-Siphon Valve or a CADD® Administration Set with either an integral or add on Anti-Siphon Valve to protect against unregulated gravity infusion that can result from an improperly attached cassette. Unregulated gravity infusion could result in death or serious injury to the patient.

Polemount Bracket recess

The optional Polemount Bracket slides into the recess on the back of the pump, allowing you to attach the pump to an IV pole.

Battery compartment

The 9 volt battery fits into this compartment. The 9 volt battery serves as the primary source of power, or as a backup when an EPS System power pack or AC Adapter is in use.

Cassette latch

This attaches the cassette (the part of the Medication Cassette™ Reservoir or CADD® Administration Set that attaches to the pump) to the pump. The pump detects whether the cassette is latched properly. Delivery will stop and an alarm will occur if the cassette becomes unlatched.

Cassette lock

This allows you to secure the cassette to the pump using the key provided. The cassette must be latched before it can be locked. In the PCA delivery mode, the cassette *must* be locked onto the pump or the pump will not run.

Downstream Occlusion Sensor (Not Shown)

The pump contains a downstream occlusion sensor. When a downstream occlusion (between pump and patient) is detected, an alarm will sound, delivery will stop, and the display will show “High Pressure.”

Upstream Occlusion Sensor (Model 6101 only; Not Shown)

The pump contains an upstream occlusion sensor. This feature may be turned on or off (see Section 5, Biomed Toolbox). When the sensor is turned on, and an upstream occlusion (between pump and fluid container) is detected, an alarm will sound, delivery will stop, and the display will show “Upstream Occlusion.”

WARNING: When the Upstream Occlusion Sensor is turned off, the pump will not detect occlusions upstream (between pump and fluid container). It is recommended that you periodically inspect the fluid path for kinks, a closed clamp, or other upstream obstructions. Upstream obstructions may result in under- or non-delivery of medications to the patient. If undetected, these occlusions could lead to death or serious injury to the patient.

Reservoir Volume Alarm (Not Shown)

Reservoir Volume is a feature that indicates when the fluid in the fluid container is low or depleted. Each time you change the fluid container, you may reset the Reservoir Volume to the originally programmed volume. Then, as medication is delivered, the Reservoir Volume automatically decreases.

Medication Cassette™ Reservoir or CADD® Administration Set: When the pump calculates that 5 ml remain in the fluid container and a “Reservoir Volume Low” message appears. This alarm recurs at every subsequent decrease of 1 ml until the Reservoir Volume reaches 0 ml, at which point the pump stops.

CADD-Prizm® High Volume Administration Set: When the pump calculates that 25 ml remain in the fluid container, beeps sound and “Reservoir Volume Low” appears. This alarm recurs at every subsequent decrease of 5 ml until the Reservoir Volume reaches 0 ml, at which point the pump stops.

The Main Screen

The main screen is the starting point for programming or viewing the pump's settings. If no keys are pressed, the display will eventually revert to the main screen. The main screen within each delivery mode displays information about the delivery status, as shown below.

PCA Delivery Mode

Power source status† Delivery mode

```

*** PCA 6210X ***
Battery Low  RUNNING
Res Vol     50.0 ml
Press NEXT to advance
  
```

“RUNNING” if the pump is running
 “DOSING” if a Demand Dose is in progress
 “STOPPED” if the pump is stopped

Continuous Delivery Mode

```

*** CONTIN 6220X ***
Battery Low  RUNNING
Res Vol     50.0 ml
Press NEXT to advance
  
```

“RUNNING” if the pump is running
 “STOPPED” if the pump is stopped
 The current Reservoir Volume
 Reminder that the NEXT key advances to programming screens

TPN Delivery Mode

```

*** TPN 6230X ***
Battery Low  RUNNING ↑
Res Vol     50.0 ml
Press NEXT to advance
  
```

“RUNNING ↑” if delivery is tapering up
 “RUNNING ↗” if delivering at the plateau rate
 “RUNNING ↓” if delivery is tapering down
 “RUNNING K” if delivering the KVO
 “RUNNING I” if immediately tapering down
 “STOPPED” if the pump is stopped

Intermittent Delivery Mode

```


*** INTERMT 6240X ***
Battery Low  DOSING
Res Vol     50.0 ml
Press NEXT to advance
  
```

“DOSING” if a dose is in progress
 “KVO” if the KVO rate is in progress
 “KVO=0” if the pump is running but no KVO is programmed
 “STOPPED” if the pump is stopped
 “DELAY” if the dose is delayed by Next Dose Start Time (KVO is delivering)

† The Power Source Status will only display when the 9 volt battery is low, unless the pump has been customized to *always* show the type of power source in use. (See Biomed Toolbox, Section 5.)

Getting Help Using the Key

For more information about a screen or message on the pump's display, press the  key to view help screens. Help screens describe what you see on the display. They may also explain why a screen or message appeared and what to do next.

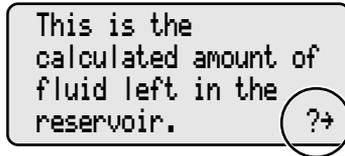

This symbol in the lower right corner means there are additional help screens. Press the  key again to see the next help screen.

- To page through all the help screens, press  repeatedly. The original screen will reappear when no further help is available.
- To exit help, press any key (other than the  key). This will bring you back to the original screen.
- If a help screen tells you to press a certain key, first exit help, then press that key.

Help screens are lock level dependent. If the pump's current lock level prevents access to a certain function, the function will not be described in the help screens.

Lock Levels

Lock levels are used to limit patient access to certain programming and operating functions. The table on the next page lists the functions that are accessible in Lock Level 0 (LL0), Lock Level 1 (LL1), and Lock Level 2 (LL2). When a function is accessible, the key associated with the function beeps when pressed. If a function is not accessible, the pump ignores the key press and a beep does not sound. Section 2, Pump Setup and Programming, describes how to change the lock level.

AutoLock

AutoLock is one of the Options. This feature automatically changes the lock level from LL0 to LL1 or LL2 when the pump is started (instead of requiring you to manually change the lock level before giving the pump to the patient). See Section 4 for more information on using AutoLock.

Security Codes

The following security codes are preset by the manufacturer for the clinician's use:

*** text removed from online version ***

WARNING: Do not disclose to the patient the pump's security codes or any other information that would allow the patient complete access to all programming and operating functions. Improper programming could result in death or serious injury to the patient.

Customizing the Security Codes

If it becomes necessary to change the Lock Level Code, Access Code, and Biomed Toolbox Code to ensure that a patient will be unable to access these features, you may customize the Lock Level Code in the Biomed Toolbox. (See Section 5.) Customizing the Lock Level Code will not affect the Clinician Bolus Code.

Lock Level Table

This table shows the features that can be accessed in each lock level. LL0 permits complete access to all programming and operating features. LL1 permits limited programming and access, and LL2 permits only minimal access.

Pump Operations and Programming	Stopped		
	LL0	LL1	LL2
Stop/Start the pump	Yes	Yes	Yes
View Help screens	Yes	Yes	Yes
Print	Yes	Yes	Yes
Reset Reservoir Volume	Yes	Yes	Yes
Reset Infusion Profile (TPN)	Yes	Yes	Yes
Change the lock level	Yes, w/code	Yes, w/code	Yes, w/code
Change the program	Yes	Within LL0 Limits†	No
Change Next Dose Start Time (INTERMT)	Yes	No	No
Clear Given amount	Yes	Yes	No
Clear Dose Counters (PCA)	Yes	Yes	No
Options			
Immediate Taper-Down (TPN)	Yes, programmable	Yes, programmable	Yes, not programmable
Prime	Yes	Yes	No
Time Remaining, view (INTERMT)	Yes	Yes	Yes
Extended History, view (PCA)	Yes	Yes	Yes
Change Delivery Modes	Yes, w/code	No	No
AutoLock	Yes	View only	View only
Time	Yes	View only	View only
Date	Yes	View only	View only
Air Detector On/Off	Yes	View only	View Only
Event Log, view	Yes	Yes	Yes
Biomed Toolbox	Yes, w/code	No	No

† In PCA and CONTIN delivery modes

Section 1: General Description

Section 2: Pump Setup and Programming

Installing a Battery

Use a new, 9 volt alkaline or lithium battery such as the DURACELL® Alkaline MN 1604, the EVEREADY® ENERGIZER® Alkaline #522 or the ULTRALIFE® Lithium U9VL battery. The pump retains all programmed values while the battery is removed. If the pump is running, you may connect an external power source to keep the pump running for 3 minutes while you change the battery.


Dispose of used batteries in an environmentally safe manner, and according to any regulations which may apply.

WARNING:


- Do not use rechargeable NiCad or nickel metal hydride (NiMH) batteries. Do not use carbon zinc (“heavy duty”) batteries. They do not provide sufficient power for the pump to operate properly, which could result in death or serious injury to the patient.
 - Always have new batteries available for replacement. If power is lost, non-delivery of drug will occur and, depending on the type of drug being administered, could result in death or serious injury to the patient.
 - There is no pump alarm to alert users that a battery has not been properly installed or has become dislodged. An improperly installed or dislodged battery could result in loss of power and non-delivery of drug and, depending on the type of drug being administered, could result in death or serious injury to the patient.
 - If the pump is dropped or hit against a hard surface, the battery door may become broken or damaged. **DO NOT USE** the pump if it has been damaged in this way because the battery will not be properly secured; this may result in loss of power, non-delivery of drug, and, depending on the type of drug being administered, death or serious injury.
-
-

To install a battery

1. Make sure the pump is stopped. Press the button on the battery door and slide the battery door forward. Remove the used battery.



2. Match the + and - markings on the new battery with the markings on the pump. Insert the battery. The pump will beep if the battery is inserted correctly.
3. Replace the battery door.

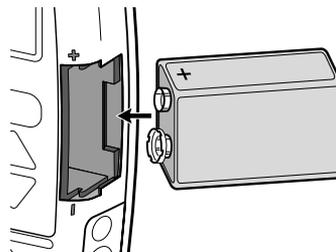

NOTE: If you put the battery in backwards, the display will remain blank. Reinsert the battery, making sure to match the + and - markings.

CAUTION: Do not store the pump for prolonged periods with the battery installed. Battery leakage could damage the pump.

NOTE:

- Battery life is dependent on the amount of medication delivered, delivery rate, battery age, temperature, frequent screen display and backlighting and frequent printing.
- At the rate of one 50 ml Medication Cassette™ Reservoir per day, alkaline batteries will usually last approximately seven days.
- The power of the battery will be quickly depleted at temperatures below +10°C (50°F).

Watching Power Up

When you install a battery, the pump will start its power up sequence during which it performs self-tests and displays programmed values. Watch for the following:

- Pump model number, last error code (“lec”), if any, and serial number (“sn”) will appear.
- The delivery modes contained in the pump and its software version will appear. Make sure the desired delivery modes are displayed.
- The display will turn completely on. Look for any stripes, which would indicate a faulty display.
- If no Air Detector is attached, “No Air Detector attached” will appear. The pump’s program screens will appear, followed by screens showing the lock level setting. AutoLock setting (if in use), Air Detector status (if an Air Detector is attached), time, and date. You may need to confirm certain settings before power up will continue. If messages appear, see the Alarms and Messages Table in Section 6 for further explanation and instructions.
- When power up is complete, “Power Up Successful” will appear, six beeps will sound, and the pump will be stopped.
- Make sure the pump is in the desired delivery mode. If not, change the delivery mode before programming (Section 4, Options).

NOTE:

- When the pump is powered up in Lock Level 0 with an Air Detector attached, the pump will automatically turn on the Air Detector (the Air Detector setting in Options will change to “Turned On.”)
- To move quickly through the power up screens, press  repeatedly. To skip the automatic review entirely, press .

Changing the Lock Level

Before programming the pump, make sure the lock level is LL0. LL0 allows the clinician to access all programming and operating functions.

To change the lock level

1. Make sure the pump is stopped.
Press **LOCK**. The current lock level will appear. (If the pump is already in the desired lock level, press **NEXT** to exit.)



Lock Level
◆ LL2

2. Press **▲** or **▼** until the desired lock level appears.



Lock Level
LL0

3. Press **LOCK** again. "000" will appear.

NOTE: If <Custom> appears on the screen, the Lock Level Code has been customized. Enter the custom Lock Level Code in the next step.



Lock Level Code
000

4. Press **▲** or **▼** until the Lock Level Code ******* (or the custom code) appears.



Lock Level Code

WARNING: Do not disclose to the patient the pump's security codes or any other information that would allow the patient complete access to all programming or operating functions. Improper programming of the pump could result in death or serious injury to the patient.

5. Press **LOCK** to set the new lock level. Watch the display to verify that the correct lock level is being entered. If you do not see this message, the lock level has not changed. Repeat the above steps.



Lock Level
LL0
<Changing...>


NOTE: To check the lock level, press **LOCK**. The current lock level will appear. To return to the screen you were on, press **NEXT**.

PCA Delivery Method

The PCA delivery method provides the following methods of delivery:

- **Continuous Rate**
- **Demand Dose**, activated by the patient
- **Clinician Bolus**, a dose activated by the clinician.

You may program each of the methods individually or in combination with each other. The following graph illustrates the combined delivery methods. Ranges and programming increments are listed in the Specifications in Section 6.

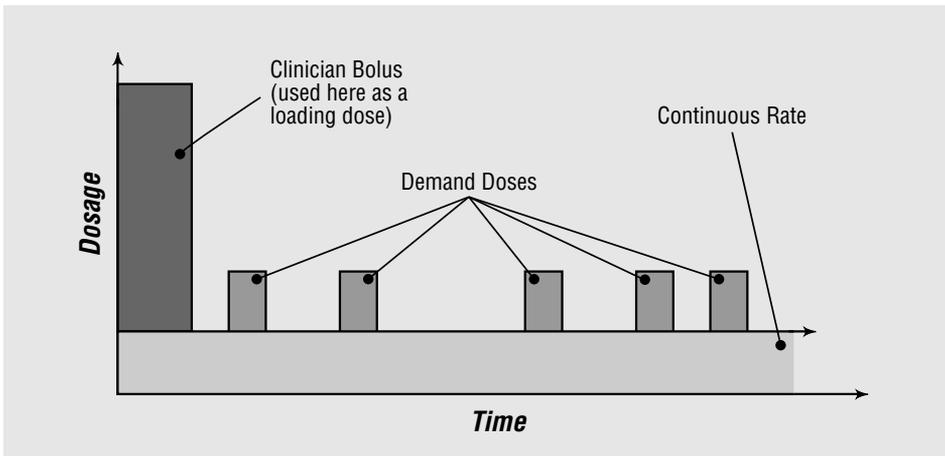

PCA Programming Screens

These are the programming screens for the PCA delivery method. Descriptions of the screens follow.

PCA Main Screen	<pre> *** PCA 6210X *** STOPPED Press NEXT to advance </pre>
Reservoir Volume	<pre> Reservoir Volume ⚡ 100.0 ml <Range: 1 - 9999> </pre>
Units	<pre> Units ⚡ Milligrams <Range: mg or ml> </pre>
Concentration (ml, mg or mcg)	<pre> Concentration ⚡ 1.0 mg/ml <Range: 0.1 - 100> </pre>
Continuous Rate	<pre> Continuous Rate ⚡ 5.00 mg/hr <Range: 0 - 30.00> </pre>
Demand Dose	<pre> Demand Dose ⚡ 2.50 mg <Range: 0 - 9.90> </pre>
Demand Dose Lockout	<pre> Demand Dose Lockout ⚡ 15 Min <Range: 5 min-24 hr> </pre>

Max. Doses per Hour

```

Max Doses Per Hour
  # 2
<Range: 1 - 4>

```

Dose Counters

```

Dose Counters
Given/Attempt: 0/ 0
since 06/08/00 10:35
Press ENTER to clear

```

(Units) Given

```

Milligrams Given
  0.00 mg
since 06/08/00 10:35
Press ENTER to clear

```

Air Detector (review)

```

Air Detector
  Required
<Review Only>

```

New Patient Marker (optional)

```

To insert New Patient
Marker and clear
Extended History press
ENTER

```

Reservoir Volume

Enter the volume of fluid contained in a filled fluid container. The Reservoir Volume value decreases as the pump delivers fluid or you use the priming feature. When you change the fluid container and reset the Reservoir Volume, the value resets to the value entered on this screen. If you do not wish to use the Reservoir Volume feature, scroll down to “Not In Use” (located before 1 and after 9999 in the range of values).

Units

Enter the programming units. Possible settings are milliliters and milligrams. Micrograms will also be one of the choices if the Micrograms settings in the Biomed Toolbox is “On.” When you change the Units, the pump requires you

to enter or verify the Continuous Rate and Demand Dose. If the units are mg or mcg, you must also enter the Concentration. Changing the Units clears the amount Given and the Extended History.

Concentration

If Units are mg or mcg, enter the concentration of drug in mg/ml or mcg/ml. When you enter a new Concentration, the pump requires you to enter a new Continuous Rate and Demand Dose.

Continuous Rate

Enter the continuous rate of medication delivery (in mg/hr, ml/hr, or mcg/hr, depending on the Units). The maximum rate is 30 ml/hr or the mg or mcg equivalent. If the prescription does not call for a Continuous Rate, enter zero.

NOTE: If you intend to run the pump in Lock Level 1 so the Continuous Rate can be varied, you should enter the maximum allowable rate while programming in Lock Level 0. After programming, you may then change to Lock Level 1 and decrease the rate to its starting value. See Programming with Upper Limits, Adjusting Doses in LL1 at the end of this section

Demand Dose

Enter the amount of drug to be delivered when the patient presses the  key (or the Remote Dose Cord button, if attached). If the prescription does not call for a Demand Dose, enter zero.

NOTE: If you intend to run the pump in Lock Level 1 so the Demand Dose can be varied, you should enter the maximum allowable dose while programming in Lock Level 0. After programming, you may then change to Lock Level 1 and decrease the dose to its starting value. See Programming with Upper Limits, Adjusting Doses in LL1 at the end of this section.

Demand Dose Lockout

If you programmed a Demand Dose, enter the minimum amount of time that must elapse between the time one Demand Dose starts and the time the next Demand Dose starts. This lockout period is unaffected by removal of the battery or stopping of the pump.

Max Doses Per Hour

This screen appears only if Max Doses Per Hour is “On” in the Biomed Toolbox. If you programmed a Demand Dose, enter the maximum number of Demand Doses allowed in any one-hour period. The possible values may be limited by the Demand Dose Lockout time you entered. If the Demand Dose Lockout is one hour or greater, this screen will not appear. The actual lockout time will be determined by either the Demand Dose Lockout or the Max Doses Per Hour, whichever is more restrictive. The Max Doses Per Hour limit is unaffected by removal of the battery or stopping of the pump.

NOTE: The number shown on this screen may be outside of the range; this can happen when the Demand Dose Lockout time is changed but the Max Doses Per Hour number is not adjusted. If you scroll through the numbers, only numbers within the range will appear.

Dose Counters

This screen appears if you programmed a Demand Dose. It shows the number of Demand Doses given and attempted since the date and time indicated, which is the last time they were cleared. (If the counters reach 999, they automatically return to zero and continue counting.) Even if these counters show zeroes, you should clear this screen during programming to update the time and date markers.

- **Given** shows the number of Demand Doses actually delivered to the patient, including doses stopped in progress.
- **Attempt** shows the total number of Demand Doses attempted by the patient while the pump was running, including doses that were delivered, locked out, and stopped in progress.

(Units) Given

This screen shows the total amount of drug delivered since the time and date indicated, which is the last time this value was cleared. The amount shown is rounded to the nearest 0.01 mg, ml, or mcg. (If this value reaches 99999.99, it automatically returns to 0 and continues counting. For concentrations of 0.5, 0.4, 0.3, 0.2 and 0.1 mg/ml, the value changes at 49999.99, 39999.99, 29999.99, 19999.99, and 9999.99 mg respectively.) The Given amount does not include drug delivered with the priming feature. Even if this screen shows zero, you should clear this screen during programming to update the time and date markers.

Air Detector Status

This screen appears only if an Air Detector is attached to the pump. It indicates whether the Air Detector is required, turned on, or turned off.

New Patient Marker

This screen appears only if the Extended History is “On” in the Biomed Toolbox. When you add a New Patient Marker, an event is added to the Event Log to indicate the pump was programmed for a new patient, and any previous information contained in the Extended History is cleared.

Options Specific to the PCA Delivery Mode

The Extended History option is available in the PCA delivery mode, which allows you to view dosing information either during a specified time period or hour by hour (see Section 4, Options).

PCA Programming Example

Medication is provided in a 100 ml Medication Cassette™ Reservoir at a concentration of 1.0 mg/ml. The patient should receive medication continuously at 5.0 mg/hr. Patient-activated doses of 2.5 mg are allowed, with a 15 minute lockout time between doses, and a maximum of 2 doses per hour.

Before programming:

- Stop the pump and change the Lock Level to LL0 as described in Section 1.
- Select the PCA delivery mode as described in Changing Delivery Modes in Section 4. If the pump is already in the PCA delivery mode, you may select it again to clear all programming screens to their default settings.

For a full description of each programming screen, see the preceding pages.

1. Begin at the main screen

```
*** PCA 6210X ***
          STOPPED
Press NEXT to advance
```

- Make sure the pump is in LL0.
- Make sure PCA and STOPPED appear on the main screen.
- Press **NEXT** to begin.

2. Enter the Reservoir Volume

```
Reservoir Volume
  † 100.0 ml
<Range: 1 - 9999>
```

- Press **▲** or **▼** to select the desired volume. (If you do not wish to use the Reservoir Volume feature, scroll down to “Not In Use” located before 1.)
- Press **ENTER**.

3. Enter the Units

To accept the current programming Units, press **NEXT**.

```

Units
  † Milligrams
<Range: mg or ml>
  
```

```

Change Units
to Milligrams?

Press Y or N
  
```

Or, to change the units:

- Press **▲** or **▼** to select the desired programming units.
- Press **ENTER**.
- Press **▲** to confirm the change.

NOTE: If the prescription calls for milliliters, enter Milliliters and skip to step 5.

4. Enter the Concentration of the drug

This screen will not appear if the units are milliliters; go to step 5.

```

Concentration
  † 1.0 mg/ml
<Range: 0.1 - 100>
  
```

```

Change Concentration
to 1.0 mg/ml?

Press Y or N
  
```

- Press **▲** or **▼** to select the desired concentration. (If you cannot select the desired concentration, it may have been turned off in the Biomed Toolbox)
- Press **ENTER**.
- Press **▲** to confirm the change.

NOTE: If you change the Concentration, you *must* enter the Continuous Rate and Demand Dose.

5. Enter the hourly Continuous Rate

```

Continuous Rate
  † 5.00 mg/hr
<Range: 0 - 30.00>
  
```

- Press **▲** or **▼** to select the desired rate.
- Press **ENTER**.

NOTE: If “Change Rate to...?” appears, you must confirm the rate because the Units or Concentration was changed, or the rate is greater

than or equal to 100 mg/hr or mcg/hr. Press **▲** to confirm, or press **▼** and re-enter the rate.

6. Enter the Demand Dose amount

Demand Dose
 ⚡ 2.50 mg
 <Range: 0 - 9.90>

- Press **▲** or **▼** to select the desired amount.
- Press **ENTER**.

NOTE: If “Change Demand Dose to...?” appears, you must confirm the dose because the Units or Concentration was changed, or the dose is greater than or equal to 100 mg or mcg. Press **▲** to confirm, or press **▼** and re-enter the dose.

7. Enter the Demand Dose Lockout time

If Demand Dose is zero, this screen will not appear; go to step 10.


Demand Dose Lockout
 ⚡ 15 Min
 <Range: 5 min-24 hr>

- Press **▲** or **▼** to select the desired lockout time between doses.
- Press **ENTER**.

WARNING: When you enter a new Demand Dose Lockout time, any lockout time in effect will be cleared. A Demand Dose could be requested and delivered immediately upon starting the pump, resulting in over-delivery, which could result in death or serious injury to the patient.

8. Enter the Max Doses Per Hour

This screen will appear only if the Max Doses Per Hour function is on. If Demand Dose is zero or the Lockout is one hour or greater, this screen will not appear; go to step 10.

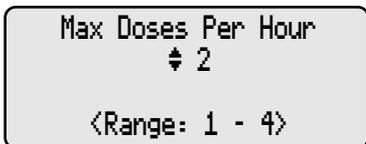


NOTE: The number shown on this screen may be outside of the range; this can happen when the Demand Dose Lockout time is changed but the Max Doses Per Hour number is not adjusted. If you scroll through the numbers, only numbers within the range will appear.

- Press **▲** or **▼** to select the maximum number of doses per hour.
- Press **ENTER**.

WARNING: When you enter a new Max Doses per Hour value, any lockout time in effect will be cleared. A Demand Dose could be requested and delivered immediately upon starting the pump, resulting in over-delivery, which could result in death or serious injury to the patient.

9. Clear the Dose Counters

If Demand Dose is zero, this screen will not appear; go to step 10.

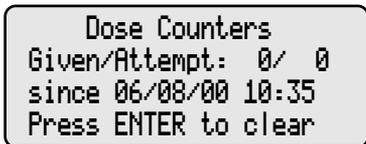

- Press **ENTER** if you wish to clear the counters; even if the counters are zero, this updates the time and date markers.

10. Clear the units Given

```

Milligrams Given
  0.00 mg
since 06/08/00 10:35
Press ENTER to clear
  
```

- Press **ENTER** if you wish to clear the amount given; even if the amount is zero, this updates the time and date markers.

11. Verify the Air Detector status

This screen will appear only if an Air Detector is installed.

```

Air Detector
Required

<Review Only>
  
```

- Make sure the setting is correct. **NOTE:** If the Air Detector is not required, this screen will show whether it is turned on or off.
- Press **NEXT** to continue. If you need to correct the Air Detector setting, see Section 4, Options.

12. Enter a New Patient Marker (optional)

This screen will appear only if the Extended History is on.

If you do not wish to add a New Patient Marker, press **NEXT**.

```

To insert New Patient
Marker and clear
Extended History press
ENTER
  
```

```

Clear Extended
History and insert
New Patient Marker?
Press Y or N
  
```

If you wish to add a New Patient Marker to the Event Log,

- Press **ENTER**.
- Press **▲Y**. This will clear the Extended History from the last patient and add a marker to the Event Log. The main screen will reappear.

13. Review the program

Press **NEXT** repeatedly to review the programming screens. If you need to reprogram a setting, press **NEXT** until the appropriate screen appears and change the setting as described in this section.

14. Prepare the Pump for the Patient

Follow the instructions for attaching a cassette, priming, changing the lock level, and attaching the pump to the patient (Section 3).


PCA: Programming with Upper Limits, Adjusting Doses in Lock Level 1

If a prescription allows for the Continuous Rate or Demand Dose to be adjusted during the course of therapy, you may wish to operate the pump in LL1. Then, when necessary, you can adjust the Continuous Rate or the Demand Dose values up to the maximum value that was programmed in LL0.

Programming the pump to use this feature

The following example shows how to set an upper Demand Dose limit of 5.00 mg with a starting value of 2.50 mg. The same procedure is used to set an upper limit and starting value on the Continuous Rate screen.


1. During initial programming in LL0, enter the **upper limit** values for the Continuous Rate and/or Demand Dose. (These will be the maximum values when the pump is in LL1.)

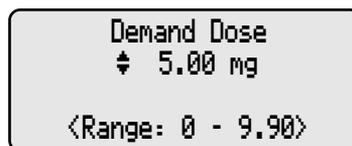

Demand Dose
⬆ 5.00 mg
<Range: 0 - 9.90>

2. After you are finished programming, change the lock level to LL1.

3. Decrease the Continuous Rate or Demand Dose to its starting value, then press (ENTER). “Range: Limited” indicates you cannot increase the value beyond the maximum programmed in LL0.

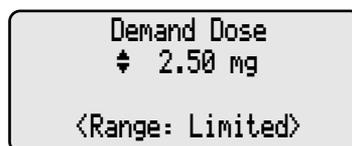


Demand Dose
⬆ 2.50 mg
<Range: Limited>

Adjusting the rate or dose while the pump is in use

If it becomes necessary to increase the Continuous Rate or Demand Dose during the course of therapy, stop the pump but *remain in LL1*.

1. Press (NEXT) until the Continuous Rate or Demand Dose screen appears.
2. Press ▲ or ▼ to select the desired value, then press (ENTER). “Range: Limited” indicates you cannot increase the value beyond the maximum.
3. Restart the pump if appropriate.

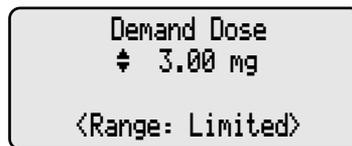

Demand Dose
⬆ 3.00 mg
<Range: Limited>

PCA: Starting a Clinician Bolus

A Clinician Bolus may be delivered in any lock level while the pump is running. It allows you to deliver a specified amount of drug, as a loading dose for example. Lockout settings have no affect on Clinician Bolus frequency. However, a Clinician Bolus cannot be started while a Demand Dose is in progress. The amount delivered decreases the Reservoir Volume and increases the Given amount, but does not add to the Dose Counters. A Clinician Bolus may be stopped in progress.

WARNING: Exercise extreme care when using the Clinician Bolus function. Since there are no limits on the frequency of delivering a bolus, and since the amount of the bolus can be set as high as 20 ml (or the mg or mcg equivalent), you should not permit the patient to become familiar with the procedure for giving a Clinician Bolus. Improper programming could result in death or serious injury to the patient.

To start a Clinician Bolus


1. Make sure the pump is running (in any lock level). Start the pump if necessary.
2. Press **LOCK**.
3. Press **▼** until the Clinician Bolus Code ******* appears on the display.
4. Press **LOCK** again.



Clinician Bolus Code

WARNING: To prevent the patient from accessing the Clinician Bolus function, do not let the patient know this code. Improper programming could result in death or serious injury to the patient.

5. Press **▲** or **▼** to select the desired amount.
6. Press **ENTER** or **DOSE**.

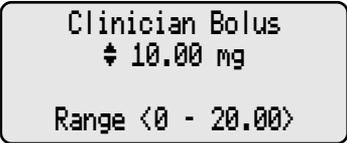


Clinician Bolus
♦ 10.00 mg
Range <0 - 20.00>

NOTE: If you enter a value of 100, a screen will appear asking you to

confirm the value. Press ▲ to confirm, or ▼ to re-enter the value.

7. The screen will show the amount decreasing as the bolus is delivered.

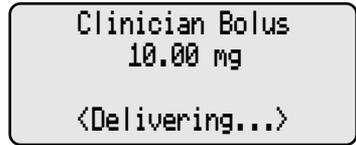

PCA: Starting a Demand Dose

If a Demand Dose has been programmed, the patient may start a Demand Dose while the pump is running. The amount delivered is added to the amount provided by the Continuous Rate. Each time the patient requests a Demand Dose, the pump will automatically add it to the Dose Counters screen. If no Demand Dose has been programmed, the pump will display the message “Dose not delivered, No Dose programmed.”

If the patient attempts to deliver a Demand Dose during the lockout time, “Dose Not Delivered, Dose Locked Out” will appear on the display and the pump will not deliver the dose. The lockout time is determined by the Demand Dose Lockout time or the Max Doses Per Hour, *whichever limits dose frequency more*. The attempt will be added to the “Attempts” counter on the Dose Counters screen.

NOTES:

- A Demand Dose cannot be started while another Demand Dose or a Clinician Bolus is in progress.
- Even if the display has automatically blanked, pressing the  key will turn the display back on and deliver a Demand Dose (if available).

To start a Demand Dose

1. Make sure the pump is running (in any lock level). Start the pump if necessary.
2. Press  (or the button on the Remote Dose Cord, if attached). Two beeps will sound and the pump will begin delivering the Demand Dose.

As the Demand Dose is delivered, the main screen will show “DOSING” in place of “RUNNING.”

```
Demand Dose
Started

NEXT to continue
```

```
*** PCA 6210X ***
Low Battery  DOSING
Res Vol      47.0 ml
Press NEXT to advance
```

PCA: Stopping a Demand Dose or Clinician Bolus

A Demand Dose or Clinician Bolus can be stopped in progress. The pump may be in any lock level. A Demand Dose that has been stopped will remain recorded on the Dose Counter screen under “Given/Attempt.”

To stop a dose while the pump is running

1. Press . One beep will sound and the message “Stop Demand Dose?” or “Stop Clinician Bolus?” will appear.
2. Press  to stop the dose and to cancel the remainder of the dose. “Demand Dose Stopped” or “Clinician Bolus Stopped” will appear.
3. When “Stop the Pump?” appears,
 - press  to remain running, or
 - press  to stop the pump.

Stop Demand Dose?

Press Y or N

Demand Dose
Stopped


Stop the Pump?

Press Y or N

Continuous Delivery Method

The Continuous delivery method provides a continuous rate of delivery in milliliters per hour.

The following graph illustrates the Continuous delivery method:

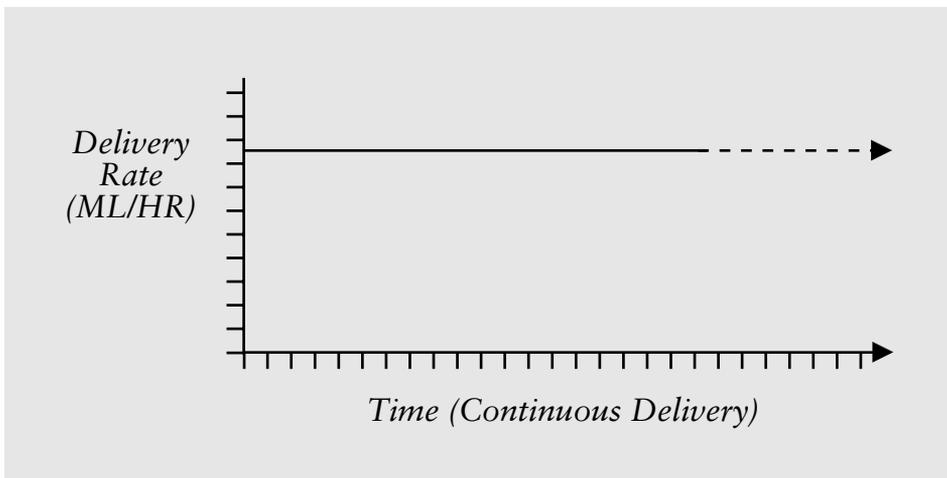

Programming Screens for Continuous Delivery

The following are the programming screens for the Continuous Delivery method. Descriptions of the screens follow.

Continuous Main Screen

```

*** CONTIN 6220X ***
                        STOPPED
Press NEXT to advance
    
```

Reservoir Volume

```

Reservoir Volume
  ⚡ 100.0 ml
<Range: 1 - 9999>
    
```

Continuous Rate

```

Continuous Rate
  ⚡ 0.5 ml/hr
<Range: 0.1 - 350.0>
    
```

Milliliters Given

```

Milliliters Given
  0.0 ml
since 01/08/00 10:35
Press ENTER to clear

```

Air Detector (review)

```

Air Detector
Required

<Review Only>

```

Reservoir Volume

Enter the volume of fluid contained in a filled fluid container. The Reservoir Volume value decreases as the pump delivers fluid or you use the priming feature. When you change the fluid container and reset the Reservoir Volume, the value resets to the value entered on this screen. If you do not wish to use the Reservoir Volume feature, select “Not In Use” (located before 1 and after 9999 in the range of values).

Continuous Rate

Enter the continuous rate of medication delivery in ml/hr. The maximum rate is 350 ml/hr.

Rates above 125 ml/hr require a CADD-Prizm® High Volume Administration Set. Rates above 250 ml/hr also require an AC Adapter or a Power Pack.

NOTE: If you intend to run the pump in Lock Level 1 so the Continuous Rate can be varied, you should enter the maximum allowable rate. After programming, you may then decrease the rate to its starting value. See Programming with Upper Limits, Adjusting Rate in LL1 at the end of this section.

Milliliters Given

This screen shows the total amount of drug delivered since the time and date indicated, which is the last time this value was cleared. The amount shown is rounded to the nearest 0.1 ml. (If this value reaches 99999.9, it automatically returns to 0 and continues counting.)

The Given amount does not include drug delivered with the priming feature. Even if this screen shows zero, you should clear this screen during programming to update the time and date markers.

Air Detector Status

This screen appears only if an Air Detector is attached to the pump. It indicates whether the Air Detector is required, turned on, or turned off.

Continuous Programming Example

Medication is provided in a 100 ml Medication Cassette™ Reservoir. The patient should receive medication continuously at 0.5 ml/hr.

Before programming:

- Stop the pump and change the Lock Level to LL0 as described in Section 1.
- Select the Continuous (CONTIN) delivery mode as described in Changing Delivery Modes in Section 4. If the pump is already in the CONTIN delivery mode, you may select it again to clear all programming screens to their default settings.

For a full description of each programming screen, see the preceding pages.

1. Begin at the main screen

```

*** CONTIN 6220X ***
                STOPPED
Press NEXT to advance
  
```

- Make sure the pump is in LL0.
- Make sure CONTIN and STOPPED appear on the main screen.
- Press **NEXT** to begin.

2. Enter the Reservoir Volume

```

Reservoir Volume
  ⚡ 100.0 ml
<Range: 1 - 9999>
  
```

- Press **▲** or **▼** to select the desired volume. (If you do not wish to use the Reservoir Volume feature, scroll down to “Not In Use” located before 1.)
- Press **ENTER**.

3. Enter the hourly Continuous Rate

```

Continuous Rate
  ⚡ 0.5 ml/hr
<Range: 0.1 - 350.0>
  
```

- Press **▲** or **▼** to select the desired rate.
- Press **ENTER**.

4. Clear the Milliliters Given

```
Milliliters Given
  0.0 ml
since 01/08/00 10:35
Press ENTER to clear
```

- Press **ENTER** if you wish to clear the milliliters given; even if the amount is zero, this updates the time and date markers.

5. Verify the Air Detector status

This screen will appear only if an Air Detector is installed.

```
Air Detector
Required

<Review Only>
```

- Make sure the setting is correct. **NOTE:** If the Air Detector is not required, this screen will show whether it is turned on or off.
- Press **NEXT** to continue. If you need to correct the Air Detector setting, see Section 4, Options.

6. Review the program

Press **NEXT** repeatedly to review the programming screens. If you need to reprogram a setting, press **NEXT** until the appropriate screen appears and change the setting as described in this section.

7. Prepare the Pump for the Patient

Follow the instructions for attaching a cassette, priming, changing the lock level, and attaching the pump to the patient (Section 3).

CONTIN: Programming with Upper Limits, Adjusting Rate in Lock Level 1

If a prescription allows for the Continuous Rate to be adjusted during the course of therapy, you may wish to operate the pump in LL1. Then, when necessary, you can adjust the Continuous Rate up to the maximum value that was programmed in LL0.

Programming the pump to use this feature

The following example shows how to set an upper Continuous Rate limit of 5.0 ml/hr with a starting value of 2.5 ml/hr.

1. During initial programming in LL0, enter the **upper limit** value for the Continuous Rate. (This will be the maximum value when the pump is in LL1.)
2. After you are finished programming, change the lock level to LL1.
3. Decrease the Continuous Rate to its starting value. “Range: Limited” indicates you cannot increase the value beyond the maximum programmed in LL0.

```
Continuous Rate
  ⚡ 5.0 ml/hr
<Range: 0 - 350.0>
```

```
Continuous Rate
  ⚡ 2.5 ml/hr
<Range: Limited>
```

Adjusting the rate while the pump is in use

If it becomes necessary to increase the Continuous Rate during the course of therapy, stop the pump but *remain in LL1*.


1. Press **NEXT** until the Continuous Rate screen appears.
2. Press **▲** or **▼** to select the desired value, then press **ENTER**. “Range: Limited” indicates you cannot increase the value beyond the maximum.
3. Restart the pump if appropriate.

```
Continuous Rate
  ⚡ 5.0 ml/hr
<Range: Limited>
```

TPN Delivery Method

The TPN delivery method allows high volume delivery of solutions, with optional tapering. Delivery can be gradually increased or “tapered up” at the beginning of the infusion profile, or it can be gradually decreased, or “tapered down” at the end of the infusion profile. When the infusion profile is completed, the pump will beep 9 times. A Keep Vein Open (KVO) rate may be delivered at the end of the infusion profile, depending on the program you have entered.

The following graph illustrates the TPN delivery method:

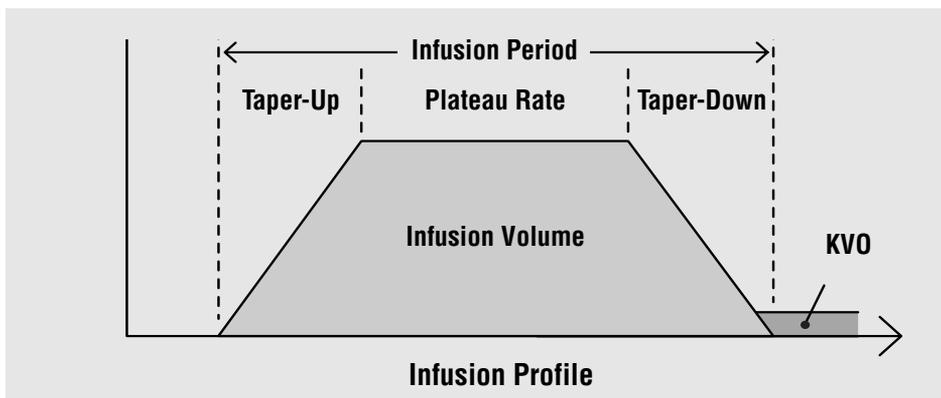

TPN Delivery

These are the programming screens for TPN Delivery. Complete descriptions of the screens follow.

TPN Main Screen

```

***  TPN 6230X  ***
                STOPPED
Press NEXT to advance
    
```

Reservoir Volume

```

Reservoir Volume
  ⚡ 1050 ml
<Range: 10.0 - 9990>
    
```

Infusion Volume

```

Infusion Volume
⚡ 1000.0 ml total
<Range: 10 - 9990>

```

Infusion Period

```

Infusion Period
⚡ 10 hrs 00 min
<Range: 3:00-99:50>

```

Taper-Up Period

```

Taper-Up Period
⚡ 1 hrs 30 min
<Range: 0:00- 9:50>

```

Taper-Down Period

```

Taper-Down Period
⚡ 1 hrs 30 min
<Range: 00:00- 8:20>

```

Plateau Rate (review)

```

Plateau Rate
    117.6 ml/hr
KVO Rate  5.0 ml/hr
<Review Only>

```

Milliliters Given

```

Milliliters Given
    0.0 ml
since 01/08/00 10:35
Press ENTER to clear

```

Air Detector (review)

```

Air Detector
  Required

<Review Only>

```

Reservoir Volume

Enter the volume of fluid contained in a filled fluid container. The Reservoir Volume value decreases as the pump delivers fluid or you use the priming feature. The Reservoir Volume programmed should be larger than the Infusion

volume, because of the fluid pumped during priming (see Priming the Tubing, Section 3), and so that automatic KVO delivery occurs at the completion of the infusion profile.

NOTE: If the programmed Reservoir Volume is greater than the Infusion Volume, KVO delivery will automatically begin when the infusion profile is complete. The KVO rate is 5 ml/hr, or 1/10th of the plateau rate. KVO delivery continues until the Reservoir Volume reaches zero, or until the pump is stopped. If the Reservoir Volume is the same as the Infusion Volume, KVO delivery will not occur at the completion of the infusion profile.

When you change the fluid container and reset the Reservoir Volume, the value resets to the value entered on this screen and the infusion profile is reset. The Reservoir Volume cannot be set to less than the programmed Infusion Volume. If you do not wish to use the Reservoir Volume feature, select “Not In Use” (located before 10.0 and after 9990 in the range of values).

Infusion Volume

Enter the total volume of fluid to be delivered. The maximum is 9990 ml. The pump calculates the Plateau Rate based on the Infusion Volume, the existing Infusion Period, and the existing Taper values. If you enter a volume that would cause the Plateau Rate to be greater than the maximum rate of 350 ml/hr or less than the minimum of 10 ml/hr, the pump will automatically lengthen or shorten the Infusion Period and may change the Taper values to accommodate the new volume. A message will appear to show that the pump is adjusting the value. You will then need to confirm the new Infusion Period or enter a different Infusion Period. Entering a new Infusion Volume resets the infusion profile so delivery will start at the beginning of the infusion period.

Infusion Period

Enter the duration for delivery of the Infusion Volume, up to 99 hours 50 minutes. The pump will automatically calculate the rate necessary to deliver the Infusion Volume you entered. You will not be able to select an Infusion Period that would cause the rate of delivery to be greater than 350 ml/hr or less than 10 ml/hr. In addition, the Infusion Period cannot be shorter than the taper periods plus 10 minutes. Entering a new Infusion Period resets the infusion profile so delivery will start at the beginning of the infusion period.

Taper-Up Period

Enter the length of time for the Taper-Up Period, up to 99 hours 40 minutes. The Taper-Up Period becomes part of the overall Infusion Period you entered. If you enter a Taper-Up Period that would cause the Plateau Rate to be greater

than the maximum rate or less than the minimum rate, the pump will automatically lengthen or shorten the Infusion Period to accommodate the new Taper-Up Period. A message will appear to show that the pump is adjusting the value. You will then need to confirm the new Infusion Period or enter a different Infusion Period. Entering a new Taper-Up Period resets the infusion profile so delivery will start at the beginning of the infusion period.

Taper-Down Period

Enter the length of time for the Taper-Down Period, up to 99 hours 40 minutes. The Taper-Down Period becomes part of the overall Infusion Period you entered. If you enter a Taper-Down Period that would cause the Plateau Rate to be greater than the maximum rate or less than the minimum rate, the pump will automatically lengthen or shorten the Infusion Period to accommodate the new Taper-Down Period. A message will appear to show that the pump is adjusting the value. You will then need to confirm the new Infusion Period or enter a different Infusion Period. Entering a new Taper-Down Period resets the infusion profile so delivery will start at the beginning of the infusion period.

Rate Display

Based on the Infusion Volume, Infusion Period, and any programmed tapering, the pump will calculate the rate of delivery that will occur during the plateau portion of the infusion profile. The calculated Plateau Rate and KVO rate (5.0 ml/hr or one tenth of the Plateau Rate) will display on this screen for review only. Rates above 125 ml/hr require a CADD-Prizm® High Volume Administration Set. Rates above 250 ml/hr also require an AC Adapter or a Power Pack.

Milliliters Given

This screen shows the total amount of drug delivered since the time and date indicated, which is the last time this value was cleared. The amount shown is rounded to the nearest 0.1 ml (If this value reaches 99999, it automatically returns to 0 and continues counting.) The Given amount does not include drug delivered with the priming feature. Even if this screen shows zero, you should clear this screen during programming to update the time and date markers.

Air Detector Status

This screen appears only if an Air Detector is attached to the pump. It indicates whether the Air Detector is required, turned on, or turned off.

Options Specific to the TPN Delivery Mode

The Immediate Taper-Down option is available in the TPN delivery mode (see Section 4, Options).

TPN Programming Example

A total of 1 liter of TPN solution must be delivered to the patient over 10 hours. The TPN bag contains 1050 ml. Delivery should taper up over 1 hour 30 minutes at the beginning of delivery and down over 1 hour 30 minutes at the end of delivery.

Before programming:

- Stop the pump and change the Lock Level to LL0 as described in Section 1.
- Select the TPN delivery mode as described in Changing Delivery Modes in Section 4. If the pump is already in the TPN delivery mode, you may select it again to clear all programming screens to their default settings.

For a full description of each programming screen, see the preceding pages.

1. Begin at the main screen

```

***  TPN 6230X  ***
                STOPPED
Press NEXT to advance
  
```

- Make sure the pump is in LL0.
- Make sure TPN and STOPPED appear on the main screen.
- Press **NEXT** to begin.

2. Enter the Reservoir Volume

```

Reservoir Volume
  † 1050 ml
<Range: 10.0 - 9990>
  
```

- Press **▲** or **▼** to select the desired volume. (If you do not wish to use the Reservoir Volume feature, scroll down to “Not In Use” located before 10.0.)
- Press **ENTER**.

3. Enter the Infusion Volume

When this screen is first displayed, the third line may show the volume left from the last infusion period. As soon as you begin scrolling to a new Infusion Volume, it will disappear.

```

Infusion Volume
⚡ 1000.0 ml total
<Range: 10 - 9990>
  
```

- Press **▲** or **▼** to select the desired volume.
- Press **ENTER**.

4. Enter the Infusion Period

When this screen is first displayed, the third line may show the amount of time left from the last infusion period. As soon as you begin scrolling to a new Infusion Period, it will disappear.

```

Infusion Period
⚡ 10 hrs 00 min
<Range: 3:00-99:50>
  
```

- Press **▲** or **▼** to select the desired Infusion Period.
- Press **ENTER**.

5. Enter the Taper-Up Period

```

Taper-Up Period
⚡ 1 hrs 30 min
<Range: 0:00- 9:50>
  
```

- Press **▲** or **▼** to select the desired Taper-Up Period.
- Press **ENTER**.

6. Enter the Taper-Down Period

```

Taper-Down Period
⚡ 1 hrs 30 min
<Range: 00:00- 8:20>
  
```

- Press **▲** or **▼** to select the desired Taper-Down Period.
- Press **ENTER**.


7. View the Calculated Rate

```

Plateau Rate
      117.6 ml/hr
KVO Rate   5.0 ml/hr
<Review Only>
  
```

- Both the Plateau Rate and the KVO Rate will be displayed. Press **NEXT** to continue.

8. Clear the Milliliters Given

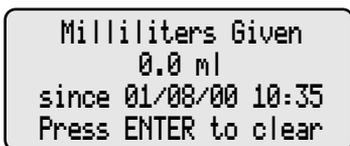

Milliliters Given
0.0 ml
since 01/08/00 10:35
Press ENTER to clear

- Press **ENTER** if you wish to clear the amount given; even if the amount is zero, this updates the time and date markers.

9. Verify the Air Detector status

This screen will appear only if an Air Detector is installed.



Air Detector
Required

<Review Only>

- Make sure the setting is correct. **NOTE:** If the Air Detector is not required, this screen will show whether it is turned on or off.
- Press **NEXT** to continue. If you need to correct the Air Detector setting, see Section 4, Options.

10. Review the program

Press **NEXT** repeatedly to review the programming screens. If you need to reprogram a setting, press **NEXT** until the appropriate screen appears and change the setting as described in this section.


11. Prepare the Pump for the Patient

Follow the instructions for attaching a cassette, priming, changing the lock level, and attaching the pump to the patient (Section 3).

TPN: Starting Daily Infusion

When a new cassette is attached to the pump at the beginning of infusion, the Reservoir Volume should be reset. This will also reset the infusion profile. To do this, follow the instructions in Section 3 for attaching a cassette and answering yes to “Reset Reservoir Volume to — ?” Then when you start the pump, delivery will begin at the start of the infusion period (illustrated below).


NOTE: Whenever the Reservoir Volume is reset, the infusion profile is also reset so the infusion will start at the beginning.

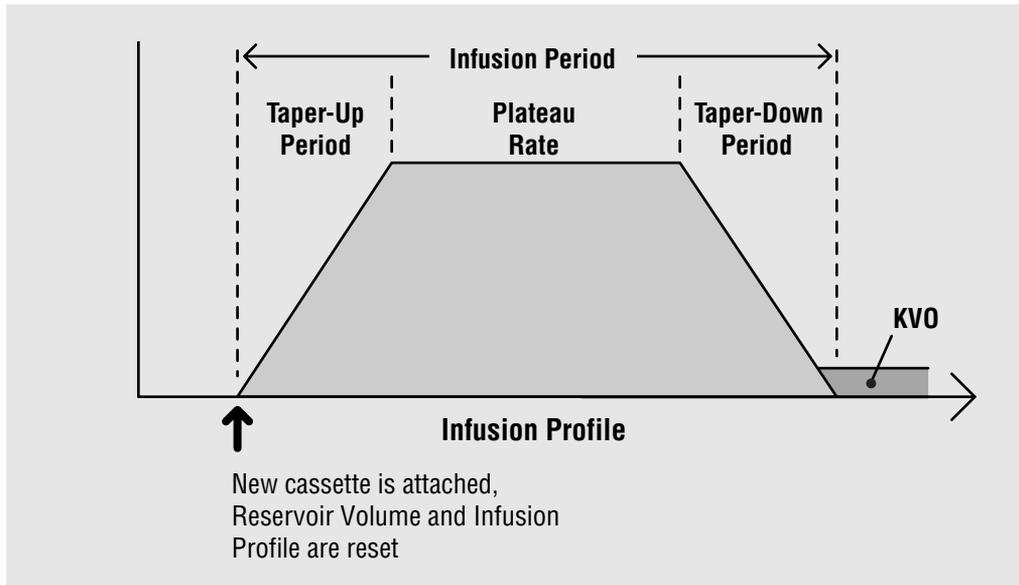

Intermittent Delivery Method

The Intermittent delivery method delivers a specified dose volume over a specified duration. You may repeat the dose in a cycle of up to 96 hours. The KVO feature allows you to deliver a minimal amount of drug between doses to maintain catheter patency. You may also delay the start of delivery using The Next Dose Start Time feature.

The following graph illustrates the Intermittent delivery method:

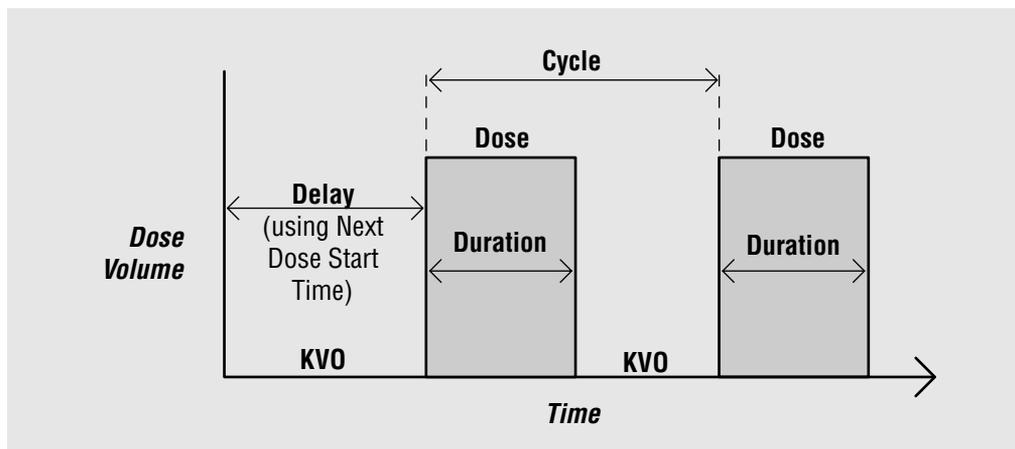

Intermittent Delivery Programming Screens

These are the programming screens for Intermittent Delivery. Complete descriptions of the screens follow.

Intermittent Main Screen

```

*** INTERMT 6240X ***
                        STOPPED
Press NEXT to advance
    
```

Reservoir Volume

```

Reservoir Volume
  ⚡ 100.0 ml
<Range: 1 - 9999>
    
```

Dose Volume

Dose Volume
 ⚡ 23.5 ml
 <Range: 0.1 - 1000>

Dose Duration

Dose Duration
 ⚡ 1 hrs 00 min
 <Range: 00:09-24:00>

Dose Cycle

Dose Cycle
 ⚡ 6 hrs 00 min
 <Range: 01:05-96:00>

KVO Rate

KVO Rate
 ⚡ 0.2 ml/hr
 <Range: 0.0 - 10>

Next Dose Start Time (optional)

Next Dose Start Time
 ⚡ 20:00 2/21/00
 <Range: See Help>

Dose Rate (review)

Dose Rate
 50.0 ml/hr
 <Review Only>

Milliliters Given

Milliliters Given
 0.0 ml
 since 01/08/00 10:35
 Press ENTER to clear

Air Detector (review)

Air Detector
 Required
 <Review Only>

Reservoir Volume

Enter the volume of fluid contained in a filled fluid container. The Reservoir Volume value decreases as the pump delivers fluid or you use the priming feature. When you change the fluid container and reset the Reservoir Volume, the value resets to the value entered on this screen. If you do not wish to use the Reservoir Volume feature, select “Not In Use” (located before 1 and after 9999 in the range of values).

Dose Volume

Enter the volume of the dose in milliliters. The maximum volume is 1000 ml. Entering a Dose Volume will automatically reset the cycle and set the Next Dose Start Time to “Immediate.” If you enter a Dose Volume that would cause the rate to be greater than the maximum rate of 350 ml/hr, the pump will automatically lengthen the Dose Duration to accommodate the new volume. You will then need to confirm the new Dose Duration or enter a different duration. The cycle may also be affected if the Dose Duration is lengthened; in this case, you would also need to confirm the new Dose Cycle or enter a different Dose Cycle.

Dose Duration

Enter the duration for delivery of the dose, up to 24 hours. You will not be able to select a duration that would cause the rate of delivery of the programmed Dose Volume to exceed 350 ml/hr. Entering a Dose Duration will automatically reset the Dose Cycle and set the Next Dose Start Time to “Immediate.” Rates above 125 ml/hr require a CADD-Prizm[®] High Volume Administration Set. Rates above 250 ml/hr also require an AC Adapter or a Power Pack.

Dose Cycle

The cycle is the time from the start of one dose to the start of the next dose. The programmable values for cycle are based on the Dose Duration. There must be at least 5 minutes between the end of one dose and the start of the next; therefore, the minimum programmable cycle is the Dose Duration plus 5 minutes. The maximum cycle is 96 hours. Entering a cycle automatically sets the Next Dose Start Time to “Immediate.”

KVO Rate

The KVO or “Keep Vein Open” rate is optional. It allows the delivery of a minimal amount of drug up to 10 ml/hr to help maintain catheter patency. If a

Next Dose Start Time is programmed, the KVO rate is active during the initial delay. The KVO rate is also active between doses.

Next Dose Start Time

The Next Dose Start Time is optional. It allows you to delay the start of delivery up to four days by allowing you to select the date and time at which the first dose should begin. The pump must be running at the selected date and time in order for delivery to begin. If a delayed start is not desired, program the Next Dose Start Time to “Immediate” so that delivery will begin as soon as you start the pump.

A Next Dose Start Time can be programmed in Lock Level 0 at any time to delay the start of the next dose, but if a dose is in progress, this will cancel the remainder of the dose. NOTE: During dosing, this screen will show “In Progress.” If a dose is stopped in progress, this screen will show “Interrupted.”

Dose Rate

This screen is for review only. It shows the rate at which the dose will be delivered based on the programmed Dose Volume and Dose Duration.

Milliliters Given

This screen shows the total amount of drug delivered since the time and date indicated, which is the last time this value was cleared. The amount shown is rounded to the nearest 0.1 ml (If this value reaches 99999, it automatically returns to 0 and continues counting.) The Given amount does not include drug delivered with the priming feature. Even if this screen shows zero, you should clear this screen during programming to update the time and date markers.

Air Detector Status

This screen appears only if an Air Detector is attached to the pump. It indicates whether the Air Detector is required, turned on, or turned off.

Options Specific to the Intermittent Delivery Mode

While a dose is being delivered, you can use the Time Remaining option to view the amount of time remaining in both the dose and the current cycle (see Section 4, Options).

Intermittent Programming Example

Medication is provided in a 100 ml Medication Cassette™ Reservoir. The patient should receive 23.5 ml dose over 1 hour. The dose should be given every 6 hours, with a 0.2 ml/hr KVO rate between doses. The first dose should begin at 8:00 PM tonight.

Before programming:

- Stop the pump and change the Lock Level to LL0 as described in Section 1.
- Select the Intermittent (INTERMT) delivery mode as described in Changing Delivery Modes in Section 4. If the pump is already in the INTERMT delivery mode, you may select it again to clear all programming screens to their default settings.

For a full description of each programming screen, see the preceding pages.

1. Begin at the main screen

```
*** INTERMT 6240X ***
                        STOPPED
Press NEXT to advance
```

- Make sure the pump is in LL0.
- Make sure INTERMT and STOPPED appear on the main screen.
- Press **NEXT** to begin.

2. Enter the Reservoir Volume

```
Reservoir Volume
  ⚡ 100.0 ml
<Range: 1 - 9999>
```

- Press **▲** or **▼** to select the desired volume. (If you do not wish to use the Reservoir Volume feature, scroll down to “Not In Use” located before 1.)
- Press **ENTER**.

3. Enter the Dose Volume

```

Dose Volume
  ⚡ 23.5 ml
<Range: 0.1 - 1000>

```

- Press **▲** or **▼** to select the desired volume.
- Press **ENTER**.

4. Enter the Dose Duration

```

Dose Duration
  ⚡ 1 hrs 00 min
<Range: 00:09-24:00>

```

- Press **▲** or **▼** to select the desired duration.
- Press **ENTER**.

5. Enter the Dose Cycle

```

Dose Cycle
  ⚡ 6 hrs 00 min
<Range: 01:05-96:00>

```

- Press **▲** or **▼** to select the desired cycle.
- Press **ENTER**.

6. Enter the KVO Rate

```

KVO Rate
  ⚡ 0.2 ml/hr
<Range: 0.0 - 10>

```

- Press **▲** or **▼** to select the desired KVO rate.
- Press **ENTER**.

7. Enter the Next Dose Start Time

```

Next Dose Start Time
  ⚡ 20:00 2/21/00
<Range: See Help>

```

- Press **▲** or **▼** to select the desired dose start time and date (or “Immediate”).
- Press **ENTER**.

```

Start next dose in
3 hrs 27 min on
2/21/00 at 20:00?
Press Y or N

```

- Verify the start time shown on the screen and press **▲** if correct. If you need to re-enter the start time and date, press **▼**.

8. Verify the Dose Rate

```
Dose Rate
50.0 ml/hr
<Review Only>
```

- The pump automatically calculates the rate of dose delivery based on the volume and duration you entered. This screen is for review only; press **(NEXT)** to continue. (If the rate is 125 ml/hr or greater, a CADD-Prizm® High Volume Administration Set must be used.)

9. Clear the Milliliters Given

```
Milliliters Given
0.0 ml
since 01/08/00 10:35
Press ENTER to clear
```

- Press **(ENTER)** if you wish to clear the amount given; even if the amount is zero, this updates the time and date markers.

10. Verify the Air Detector status

This screen will appear only if an Air Detector is installed.

```
Air Detector
Required
<Review Only>
```

- Make sure the setting is correct. **NOTE:** If the Air Detector is not required, this screen will show whether it is turned on or off.
- Press **(NEXT)** to continue. If you need to correct the Air Detector setting, see Section 4, Options.

11. Review the program

Press **(NEXT)** repeatedly to review the programming screens. If you need to reprogram a setting, press **(NEXT)** until the appropriate screen appears and change the setting as described in this section.


12. Prepare the Pump for the Patient

Follow the instructions for attaching a cassette, priming, changing the lock level, and attaching the pump to the patient (Section 3).

INTERMT: Stopping the Pump During the Cycle

Stopping the pump *during the KVO* will not affect the start time of subsequent doses.

Stopping the pump *while a dose is in progress* will shift all subsequent doses by the amount of time the pump is stopped (illustrated below).

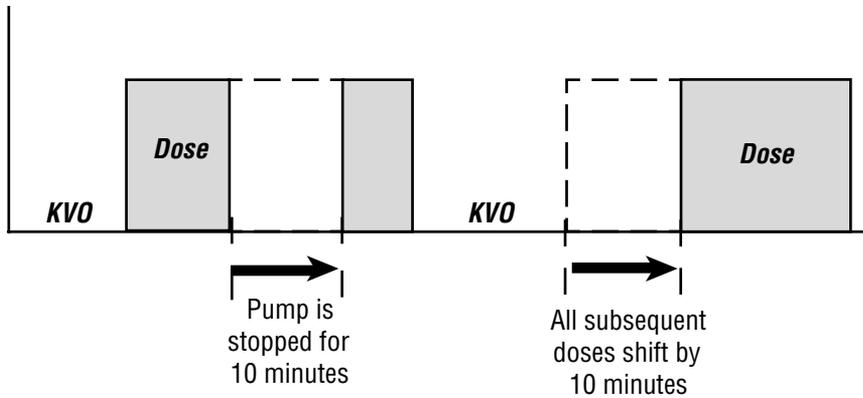

If you wish to make up for the lost time in the cycle, *it is recommended that you wait until the current dose is completed*. (To determine the amount of time remaining in the current dose, use the Time Remaining Option described in Section 4.) Then stop the pump, change to Lock Level 0, and reprogram the Next Dose Start Time.

Resuming the Dose

To resume delivery of a dose that has been stopped in progress, simply restart the pump.

Resetting the Cycle

If you wish to reset the cycle, stop the pump during KVO, change to LL0, and reprogram the Next Dose Start Time.

If a dose has been stopped in progress and you wish to cancel the current dose and reset the cycle, make sure the pump is in Lock Level 0. The Next Dose Start Time screen should show “Interrupted”. Reprogram the Next Dose Start Time. This will cancel the remainder of the dose, and the next cycle will start at the time you selected.

Section 3: Operating the Pump


Removing a Cassette

WARNING: Always close the fluid path tubing with the clamp before removing the cassette from the pump to prevent unregulated gravity infusion, which could result in death or serious injury to the patient.


1. Close the tubing clamp.
2. If the cassette is locked, insert the key and turn the lock clockwise one-quarter turn until it stops.



3. Use a coin or the side of the key to unlatch the cassette. Insert the coin or the side of the key into the slot and turn clockwise until the latching button pops out.



4. Remove the cassette hooks from the pump hinge pins.

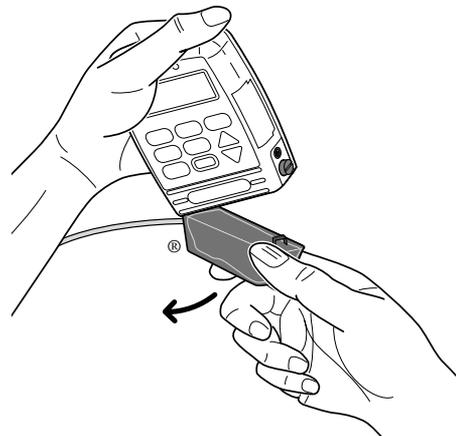

Attaching a Cassette

Obtain a new, filled Medication Cassette™ Reservoir, or CADD® Administration Set attached to a nonvented, flexible IV bag. Refer to the instructions for use supplied with the product for information on preparing the product for use.


Before you attach a new cassette, make sure a battery is installed in the pump. If a battery is installed, the pump will automatically display screens which allow you to verify the type of cassette (on the Model 6101, the screen also indicates whether the upstream occlusion sensor is on or off), reset the Reservoir Volume, prime the fluid path (depending on the lock level), change the lock level (if AutoLock is not in use and the lock level is LL0), and/or start the pump.

NOTE: You can access this sequence of screens even when you are not attaching a cassette. With the pump stopped and the main screen displayed, press **ENTER** to display the sequence beginning with verifying the type of cassette.

CAUTION: If you are using a Medication Cassette™ Reservoir in which the medication is frozen, thaw at room temperature only. *Do not heat in a microwave oven* as this may damage the product and cause leakage.

To attach the cassette to the pump


1. Clamp the tubing. Insert the cassette hooks into the hinge pins on the pump.
2. Place the pump upright on a firm, flat surface. Press down so the cassette fits tightly against the pump.
3. Insert a coin or the side of the key into the latch button, push in, and turn counterclockwise until the mark on the latch lines up with the solid dot and you feel the button click into place. A message will appear on the display so you can verify the type of cassette you

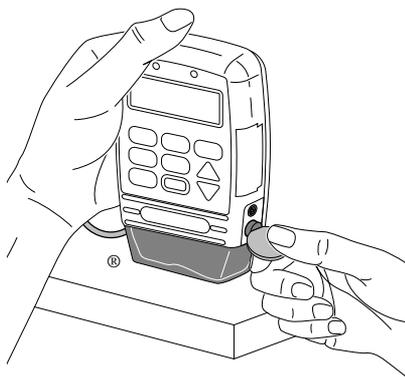

have attached (Admin Set, High Volume Admin Set, or Reservoir).


4. If appropriate, insert the pump key into the lock and turn counterclockwise until the white mark lines up with the solid dot. The message “Cassette Locked” will appear on the display. Press **NEXT**.

NOTE: In the PCA delivery mode, The cassette **must be locked** in order to start the pump.




WARNING: Attach the cassette properly. An improperly attached or detached cassette could result in unregulated gravity infusion of medication from the fluid container or a reflux of blood, which could result in death or serious injury to the patient.

You must use a CADD® Extension Set with Anti-Siphon Valve or a CADD® Administration Set with either an integral or an add on Anti-Siphon Valve to protect against unregulated gravity infusion that can result from an improperly attached cassette.



5. Gently twist and pull on the cassette to make sure it is firmly attached.
6. If “Reset Reservoir Volume to...?” appears,
 - Press ▲ to reset Reservoir Volume to the value shown, or
 - Press ▼ to retain the current value.

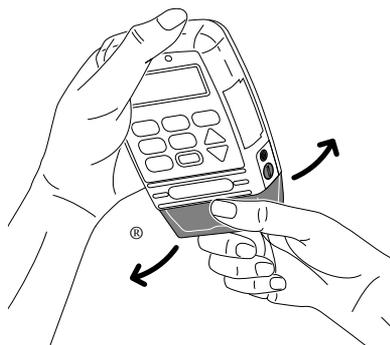

NOTE: If this screen does not appear, Reservoir Volume may already be reset.

Reset Reservoir
Volume to 100.0 ml?
Press Y or N

If this message appears, the pump is in the TPN delivery mode and Reservoir Volume is not in use. Press ▲ to reset the infusion profile.

Reset Infusion
Profile?
Press Y or N

7. If you have reset the Reservoir Volume and the pump is in the TPN delivery mode, “Infusion Profile has been reset” will also appear.

Infusion Profile
has been reset

Go to the next page.

Priming the Tubing and Connecting to the Patient

If the lock level is LL0 or LL1 when you attach a cassette, “Prime Tubing?” will appear in the sequence of screens. Prime the tubing *before* connecting it to the patient’s infusion set or indwelling catheter.

Prime Tubing?

Press Y or N

If the lock level is LL2, you cannot use the priming feature; skip to step 5 in the procedure below.

NOTE: If you are not changing the cassette but wish to prime the fluid path, you may use the Prime Option described in Section 4.

WARNING: Do not prime the fluid path with the tubing connected to a patient as this will result in over-delivery of medication, which could cause death or serious injury to the patient.

1. When “Prime Tubing?” appears, press **▲**.
2. Make sure the tubing is disconnected from the patient and the tubing clamp is open.
3. Press and hold the **▲** key until the tubing is fully primed or until priming stops.

Prime Tubing?

Press Y or N

Disconnect tubing
from patient
Open clamps
Hold Y to prime

Priming...
0.1 ml

Hold Y to prime

NOTE: Fluid delivered during priming is subtracted from the Reservoir Volume, but is not added to the Given screen since this fluid is not delivered to the patient.

4. If the tubing is not yet fully primed, press **▲** and repeat step 3.

Continue Priming?

Press Y or N


When the tubing is fully primed, press **▼** to exit priming.

5. If an Air Detector is in use, go to Inserting the Tubing into the Air Detector. If not, connect the tubing to the patient's infusion set or indwelling catheter and go to Setting the Lock Level for the Patient.

Inserting the Tubing into the Air Detector

WARNING: When the Air Detector is not installed, or is installed but turned off, the pump will not detect air in the fluid path. It is recommended that you periodically inspect the fluid path and remove any air to prevent air embolism. Air embolism could cause death or serious injury to the patient.

1. If the Air Detector is in use, open the Air Detector door and thread the tubing through the groove.
2. Close the door, making sure the tubing does not get pinched or kinked.
3. Connect to the patient's infusion set or indwelling catheter.

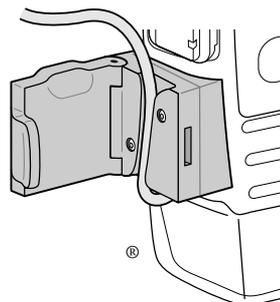

WARNING: Ensure that the entire fluid path is free of all air bubbles before connecting to the patient to prevent air embolism. Air embolism could cause death or serious injury to the patient.

NOTE: If the fluid path contains an air eliminating filter, it is acceptable for air bubbles to be present on the vent side of the filter.

4. If AutoLock is in use, or if the pump is in LL1 or LL2, "Start the Pump?" will appear; go to Starting the Pump.

If AutoLock is not in use and the lock level is LL0, the pump will prompt you to manually change the lock level; the screen at right will appear.

A screenshot of a monochrome LCD display. The text on the screen reads: "AutoLock not in use. Change Lock Level from LL0? Press Y or N". The text is arranged in four lines, with "AutoLock not in use." on the first line, "Change Lock Level" on the second, "from LL0?" on the third, and "Press Y or N" on the fourth.

```
AutoLock not in use.  
Change Lock Level  
from LL0?  
Press Y or N
```

Go to the next page.


Setting the Lock Level for the Patient

If AutoLock is not in use and the lock level is LL0 when you attach a cassette, the message “AutoLock not in use / Change Lock Level from LL0?” will appear to allow you to set the lock level to LL1 or LL2. The lock level must be reset to LL1 or LL2 to prevent the patient from having complete access to all programming and operating functions. For detailed information on lock levels, see Section 1.

NOTE: You may change the lock level at any time by stopping the pump and pressing . Then begin with step 2 below.

To change the lock level

1. With this message displayed, press . (If you do not wish to change the lock level at this time, press  and go to the next page.)

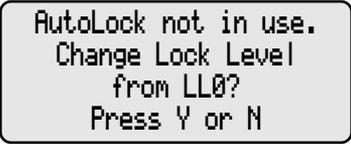

2. The current lock level will appear.



3. Press  or  until the desired lock level (LL1 or LL2) appears.



4. Press  again. “000” will appear.



NOTE: If <Custom> appears, the Lock Level Code has been customized. Use the custom Lock Level Code in the next step.

5. Press  or  until the Lock Level Code **** (or custom code) appears.



WARNING: Do not disclose to the patient the pump’s security codes or any other information that would allow the patient complete access to all programming and operating functions. Improper programming could result in death or serious injury to the patient.

6. Press **LOCK** to set the new lock level. Watch the display to verify that the correct lock level is being entered.



Starting the Pump

1. This is the last screen to appear when you attach a cassette. If the fluid path is free of air and the tubing is attached to the patient, press  to start the pump.
2. “Starting Pump” will appear.

The pump will review the program, lock level, AutoLock setting, time, and date. If AutoLock is in use, “AutoLock is changing lock level to (LL1 or LL2)” will appear.

Start the Pump?

Press Y or N

Starting Pump...

After the automatic review, the green indicator light will blink and fluid delivery will begin as programmed.

Stopping the Pump

When the pump is stopped, no delivery occurs. “STOPPED” appears on the main screen and the amber indicator light blinks.

To stop the pump

1. Press .

PCA Mode Only: If a Demand Dose or Clinician Bolus is in progress, “Stop Demand Dose?” or “Stop Clinician Bolus?” will appear. Press  to stop the dose.

2. When “Stop the Pump?” appears, press .

Stop Demand Dose?

Press Y or N

Stop the Pump?

Press Y or N

Resetting the Reservoir Volume

Normally, when you lock a cassette onto the pump as described in this section, a series of messages lead you through resetting the Reservoir Volume, priming the tubing, (except in LL2), and starting the pump.

You can, however, reset the Reservoir Volume without changing the cassette using the Reservoir Volume programming screen. The pump may be in any lock level.

NOTE: In the TPN delivery mode, resetting the Reservoir Volume also resets the infusion profile so delivery will start at the beginning of the infusion period when you start the pump.

Resetting Reservoir Volume without changing the cassette

1. Stop the pump.
2. Press **NEXT** to display the Reservoir Volume screen.
3. Press **ENTER**.
4. If this message appears, press **Y** to reset the Reservoir Volume. (If this message does not appear, the Reservoir Volume may already be reset.)

```
Reservoir Volume
  29.2 ml
<Range: Limited>
```

```
Reset Reservoir
Volume to 100.0 ml?
Press Y or N
```

If this message appears, the pump is in the TPN delivery mode and Reservoir Volume is not in use. Press **Y** to reset the Infusion Profile.

```
Reset Infusion
Profile?
Press Y or N
```

5. If you have reset the Reservoir Volume and the pump is in the TPN delivery mode, you will also see “Infusion Profile is being reset.”

Section 4: Options


Overview: Accessing Options

The Options menu allows access to other pump features and settings. The availability of an Option may depend on the pump's delivery mode, lock level, Biomed Toolbox settings, the presence of an Air Detector, and whether the pump is running or stopped. (For more information about the Communications option, refer to the product literature supplied with the CADD-Diplomat™ Communications System.)

To access Options

1. Start at any screen and press **OPTIONS**.
2. Use **▲**, **▼** or **OPTIONS** to page through the Options. To select an Option, make sure it is displayed on the Options Menu and press **ENTER**.
3. To exit the Options Menu, press **NEXT** until you return to the main screen.

The **⚡** symbol means you may use the **▲** or **▼** key to see more Options.

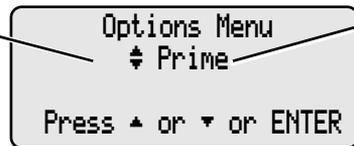

Options appear here. In this example, the "Prime" option is shown. To select the option shown, press **ENTER**. To see other options, press **▲**, **▼** or **OPTIONS**.

Immediate Taper-Down: TPN

This option is available in the **TPN delivery mode only**. It allows you to stop infusion early by immediately tapering down. If the pump is in LL0 or LL1, the Taper-Down Period can be changed from its originally programmed value, even if it is 0. You can select a Taper-Down Period that is equal to or less than the time remaining in the infusion profile. If the pump is in LL2, you can use the Immediate Taper-Down Option, but you cannot change the Taper-Down Period.

To access the Immediate Taper-Down option:

- the pump must be running
- the pump must be delivering at the plateau rate
- there must be at least 10 minutes left in the Infusion Period

IMPORTANT: Once you answer yes to the message in step 3 below, you will not be able to restart delivery of the plateau rate without resetting the Infusion Period.

1. Keep the pump running. Press **OPTIONS**.

2. If necessary, press **▲** or **▼** until “Immediate Taper-Down” appears. Press **ENTER**.

```
Options Menu
◆ Immediate Taper-Down
Press ▲ or ▼ or ENTER
```

3. *If the pump is in LL0 or LL1*, press **ENTER** to accept the current Taper-Down Period displayed.

```
Immediate Taper-Down
◆ 1 hrs 00 min
<Range 00:00-01:30>
```

Or,

Press **▲** or **▼** to select the desired Taper-Down period, then press **ENTER**. Press **▲** to confirm the period.

```
Immediate
Taper Down Period
    20 min?
Press Y or N
```

If the pump is in LL2, this message will appear. Press **▲** to begin tapering down.

```
Begin Immediate Taper
Down? Taper equals
    1 hrs 00 min
Press Y or N
```

Prime

The Prime Option is used in all delivery modes to pump fluid through the fluid path to remove air bubbles prior to connecting to the patient. The pump must be stopped and in LL0 or LL1 to prime.

Fluid delivered with the priming feature is subtracted from the Reservoir Volume value, but is not added to the amount Given (since this fluid is not delivered to the patient). Priming is not allowed when the Reservoir Volume value is 0.0 ml.

WARNING: Do not prime the fluid path with the tubing connected to a patient as this will result in over-delivery of medication or air embolism, which could result in death or serious injury to the patient.

1. Make sure the pump is stopped and in LL0 or LL1.

2. Press **OPTIONS**.

If necessary, press **▲** or **▼** until “Prime” appears. Then press **ENTER**.

3. Make sure the tubing is disconnected from the patient and the clamp is open.

4. Press and hold the **▲** key to prime. If a cassette is attached, the volume primed will appear on the screen. When finished, release the **▲** key.

5. If the tubing is not yet fully primed, press **▲** and repeat step 4.

When the tubing is fully primed, press **▼** to exit priming.

```
Options Menu
┆ Prime
Press ▲ or ▼ or ENTER
```

```
Disconnect tubing from
patient
Open clamps
Hold Y to prime
```

```
Priming...
0.1 ml
Hold Y to prime
```

```
Continue Priming?
Press Y or N
```

NOTE: If a cassette is not attached when the Prime feature is used, the Reservoir Volume value will not be affected by the amount primed.

Time Remaining: Intermittent

This option is available in the **Intermittent delivery mode only**. It allows you to view the time remaining in the current dose if one is being delivered and the time remaining in the cycle. The pump may be running or stopped and in any lock level.

1. Press **OPTIONS**.

If necessary, press **▲** or **▼** until “**Time Remaining**” appears. Then press **ENTER**.

```
Options Menu
⚡ Time Remaining
Press ▲ or ▼ or ENTER
```

2. “Dose” shows the number of hours and minutes remaining in the dose that is currently being delivered.

```
Time Remaining
Dose      0 hrs 30 min
Cycle     5 hrs 30 min
```

“Cycle” shows the number of hours and minutes remaining in the current cycle (the time that must elapse until the next dose starts).

NOTE: If dashes appear in place of times, the start of the dose has been delayed by the Next Dose Start Time, and fluid is being delivered at the KVO rate (if programmed).

```
Time Remaining in:
Dose:   -- hrs -- min
Cycle:  -- hrs -- min
NEXT to continue
```

Extended History, Viewing: PCA

The Extended History is available in the **PCA delivery mode only**. It allows you to view dose information for the past 48 hours, including doses given and attempted, and the amount delivered. The pump may be running or stopped and in any lock level. You may select from two types of views:

- **Patient Review** gives a summary of the pump’s current settings, the number of doses given and attempted, and the amount delivered, starting at a date and time you specify.
- **Doses Hour by Hour** allows you to page back through summaries for each one hour period, showing the number of doses given and attempted.



Both views show dose information for the past 48 hours, unless a New Patient Marker has been added, or the Units, Time, or Date have been changed. Dose information previous to any of these events will not appear.

NOTE: If the Extended History option does not appear, it has been turned off in the Biomed Toolbox.

To view the Extended History

These steps describe how to view the Extended History. You can also print the Extended History. (See Section 3.)

1. Press **OPTIONS**. (Any screen may be displayed.)
2. Press **▲** or **▼** until “Extended History” appears, then press **ENTER**.
3. Press **▲** or **▼** to select “Patient Review” or “Doses Hour by Hour,” then press **ENTER**.

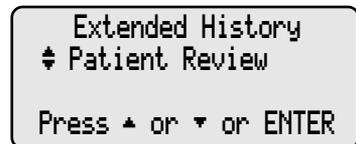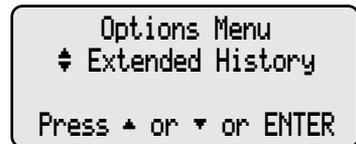

Follow the instructions for the appropriate screen on the next page.

Patient Review

1. Press ▲ or ▼ to select the start time and date, then press **ENTER**.

NOTE: All start times begin on the hour.

```
Review Start Time
* 10:00 06/07/00

Press ▲ or ▼ or ENTER
```

2. The first screen, “Pump Settings 1” will appear. Press ▲ to page forward through the Patient Review screens. Press ▼ to page backward.

```
Patient Review
* Pump Settings 1
Res Vol      60.0 ml
```

3. When finished, press **NEXT** to return to the Extended History screen.

NOTE: An asterisk (*) next to a value indicates that it applies only to the selected time period; it may not match the corresponding value in the programming screen. For example, “*Given” only reflects doses given during the selected time period, and may not match the “Given” value on the Dose Counters screen.

Doses Hour by Hour

1. After you select Doses Hour by Hour, the number of doses given and attempted during the *current hour* will appear.

- Press ▼ to page back through hours.
- Press ▲ to page forward.

```
Doses Hour by Hour
*10:00-10:59 06/08/00
*Given          1
*Attempted      2
```

2. When finished, press **NEXT** to return to the Extended History screen.

Change the Delivery Mode

The CADD-Prizm® pump contains four delivery modes: PCA, CONTIN, TPN, INTERMT. (The pump also contains a Communications mode; for more information, refer to the product literature accompanying the CADD-Diplomat™ Communications System.) To change the mode, you must know the Access Code (Lock Level Code plus 10). When you change the mode, the program will revert to the default settings, and the Event Log will clear. Therefore, you may wish to print the Event Log before changing the mode. Other Options settings will not be affected.

To change the delivery mode

The pump must be stopped and in LL0.

1. Press **OPTIONS**.

Press **▲** or **▼** until “Delivery Modes” appears, then press **ENTER**.

```
Options
  ↓ Delivery Modes
Press ▲ or ▼ or ENTER
```

2. Press **▲** or **▼** until the Access Code **** text omitted ****. Then press **ENTER**.

```
Access Code
  ***
```

**** text omitted from online version ****

3. Press **▲** or **▼** to select the desired delivery mode. Then press **ENTER**.
4. Press **▲** to confirm the change.

```
Select
  ↓ CONTIN 6220X
Press ▲ or ▼ or ENTER
```

The pump will go through the power up sequence in the new delivery mode. If messages appear, refer to the table in Section 6 or press **?** for help.

```
Change Delivery Mode
to CONTIN 6220X?
Press Y or N
```

5. After the power up sequence, this message will appear followed by the first programming screen in the new delivery mode.

```
Pump is ready to
program
NEXT to continue
```

AutoLock

The **AutoLock** Option is available in all delivery modes. It automatically changes the lock level from **LL0** to **LL1** or **LL2** when the pump is started, instead of requiring you to manually change the lock level before giving the pump to the patient. AutoLock may be set to LL1, LL2, or Not In Use.

AutoLock takes effect when you start the pump in LL0 only. It *will not* change the lock level if you set the lock level to LL1 or LL2 manually before starting the pump; the AutoLock will not override your setting.


IMPORTANT: Changing the AutoLock setting is not the same as changing the lock level. The AutoLock setting specifies the lock level that will be set when the pump is started in LL0. To manually change the pump's lock level, see Section 1, Changing the Lock Level.

To view or change the AutoLock setting

To view the setting, the pump may be in any lock level. To change the setting, the pump must be stopped and in LL0.

1. Press **OPTIONS**.


Press **▲** or **▼** until “AutoLock” appears, then press **ENTER**.

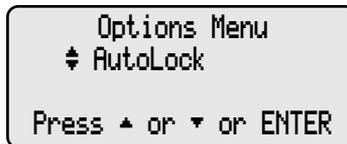

2. The *current* AutoLock setting will appear.

- To leave the setting unchanged and return to the Options menu, press **NEXT**.

- To change the setting, press **▲** or **▼** to select the desired lock level. (To turn off AutoLock, set it to “Not In Use.”) Then press **ENTER**.

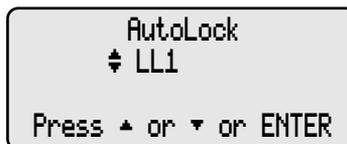

3. Press **▲** to confirm the change.



Time

The **Time** Option shows the time of day in 24-hour (military) time according to the pump's internal clock. The clock is powered by a separate, internal battery which retains the time even when the 9 volt battery is removed. The time is used to record the time of events in the Event Log.

WARNING: (PCA delivery mode) If Demand Doses are currently locked out, changing the Time will cancel the lockout period. This will allow a Demand Dose to be requested and delivered as soon as the pump is restarted, resulting in over-delivery, which could result in death or serious injury to the patient.

NOTE: Changing the time will clear the Extended History in the PCA delivery mode.

To change the Time of Day

To view the setting, the pump may be in any lock level. To change the setting, the pump must be stopped and in LL0.

1. Press **OPTIONS**.

Press **▲** or **▼** until "Time" appears with the time setting.

```
Options Menu
  ◆ Time   14:45
Press ▲ or ▼ or ENTER
```

2. To change the setting, press **ENTER**.

A message will appear notifying you of other settings that will be affected by changing the time. This message will clear in a few seconds.

```
Changing time will
clear Extended
History and reset
dose lockout time
```

3. Press **▲** or **▼** to select the desired time in **24-hour military time**, then press **ENTER**.

```
Time of Day
  ◆ 15:45
Press ▲ or ▼ or ENTER
```

4. Press **▲** to confirm the change.

```
Change Time to
  15:45?
Press Y or N
```

Date

The **Date** Option should reflect the current date. This feature is used to record the date of events in the Event Log.

WARNING: (PCA delivery mode) If Demand Doses are currently locked out, changing the Date will cancel the lockout period. This will allow a Demand Dose to be requested and delivered as soon as you restart the pump, resulting in over-delivery, which could result in death or serious injury to the patient.

NOTE: Changing the date will clear the Extended History in the PCA delivery mode.

To change the Date

To view the setting, the pump may be in any lock level. To change the setting, the pump must be stopped and in LL0.

1. Press **OPTIONS**.

Press **▲** or **▼** until “Date” appears with the date setting.

```
Options Menu
  ⚡ Date 02/20/00
Press ▲ or ▼ or ENTER
```

2. To change the setting, press **ENTER**.

A message may appear to notify you of other settings that will be affected by changing the date. This message will clear in a few seconds.

```
Changing date will
clear Extended
History and reset
dose lockout time
```

3. Press **▲** or **▼** to select the date, then press **ENTER**.

```
Date
  ⚡ 05/23/00
Press ▲ or ▼ or ENTER
```

4. Press **▲** to confirm the change.

```
Change Date to
  05/23/00?
Press Y or N
```

Air Detector On/Off

The **Air Detector** Option controls whether the Air Detector is turned on or off. This option appears in the menu only if an Air Detector is installed on the pump and is not required. (A setting in the Biomed Toolbox controls whether an Air Detector is required. If the Air Detector is required, you are not allowed to turn it off and this option will not appear in the menu.)

The Air Detector Option can be set to “Turned On” or “Turned Off.” If the Air Detector is turned on, an alarm will sound when air is detected in the fluid path. (See Section 6 for Air Detector specifications.) When the Air Detector is first attached to the pump, the Air Detector screen defaults to “**Turned On.**” This screen also changes to “Turned On” each time the pump powers up in Lock Level 0.

For certain therapies, it may be desirable to turn off the Air Detector (for example, for epidural infusion or subcutaneous infusion).

WARNING: When the Air Detector is installed but turned off, the pump will not detect air in the fluid path. It is recommended that you periodically inspect the fluid path and remove any air to prevent air embolism, which could result in death or serious injury to the patient.

To change the Air Detector setting

To view the setting, the pump may be in any lock level. To change the setting, the pump must be stopped and in LL0.

1. Press **OPTIONS**.
Press **▲** or **▼** until “Air Detector” appears, then press **ENTER**.
2. The current setting will appear.
To change the setting, press **▲** or **▼** to select the desired setting, the press **ENTER**.
3. Press **▲** to confirm the change.

```
Options Menu
┆ Air Detector
Press ▲ or ▼ or ENTER
```

```
Air Detector
┆ Turned On
Press ▲ or ▼ or ENTER
```

```
Change Air Detector to
Turned On?
Press Y or N
```

Event Log, Viewing

The **Event Log** records the following types of events: dose delivery, alarms, errors, power source changes, cassette changes, changes to pump programming or settings. The pump records the date and time of each event, and lists events in order starting from the most recent through the last 500 events or the last delivery mode change.

The pump may be running or stopped and in any lock level to view the Event Log.

To view the Event Log

1. Press **OPTIONS**.
2. Press **▲** or **▼** until “Event Log” appears, then press **ENTER**.
3. To view the events:
 - Press **▲** to page forward through events.
 - Press **▼** to page backward through events.
4. When finished, press **NEXT** to return to the Options Menu.

```
Options Menu
↓ Event Log
Press ▲ or ▼ or ENTER
```

```
Event Log Entry
↓ 06/01/00 at 10:35
9 volt battery
removed
```

Section 5: Biomed Toolbox

Overview: Accessing the Biomed Toolbox

The Biomed Toolbox contains pump configurations that are less frequently changed. The Biomed Toolbox is accessible only when the pump is stopped and in Lock Level 0.

To Access the Biomed Toolbox Menu

1. Press **OPTIONS**. Press **▲** or **▼** until “Biomed Toolbox” appears, then press **ENTER**.
2. Press **▲** or **▼** until the Biomed Toolbox Code ******** appears ********
**** omitted ****. Then press **ENTER**.

**** text omitted ****

3. Press **▲** or **▼** to select the setting you wish to view or change, then **ENTER**. Follow the instructions in this section for the appropriate screen.

NOTE: To leave a Biomed Toolbox setting unchanged, press **NEXT**.

```
Options Menu
  ↓ Biomed Toolbox
Press ▲ or ▼ or ENTER
```

```
Biomed Toolbox Code
  ***
```



```
Biomed Toolbox Menu
  ↓ Micrograms  [ ]
Press ▲ or ▼ or ENTER
```

Micrograms On/Off (PCA Only)

This screen allows you to turn on or turn off micrograms. If micrograms are off, only milliliters and milligrams will be available for programming in the Units screen.

NOTE: If the Units programming screen is set to micrograms, you cannot turn them off. You will first need to change the Units screen to milligrams or milliliters, then return to this screen to turn off micrograms.

1. At the Biomed Toolbox Menu, press  or  until “Micrograms” appears. If an X appears in the box (■), Micrograms are currently on.
2. To change the setting, press . Press  or  to select the desired setting, then press .

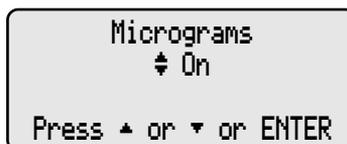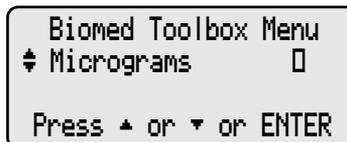


Concentration Customization (PCA Only)

This screen allows you to select the concentrations that will be available for programming in the Concentration screen (mg/ml or mcg/ml). You may turn on or turn off all concentrations, then selectively turn on or turn off individual concentrations. For example, if only three concentrations will be used, you can turn off all concentrations, then turn on those three concentrations. **At least one concentration must be on.**

Since you cannot turn off the currently programmed concentration, you may want to change the Units programming screen to milliliters before customizing concentrations.

NOTE: Even if Micrograms have been turned off (see **Micrograms On/Off** above), you can customize Microgram concentrations.

1. At the Biomed Toolbox Menu, press  or  until “Custom Conc” appears. If an X appears in the box, concentrations for either mg or mcg are currently customized.

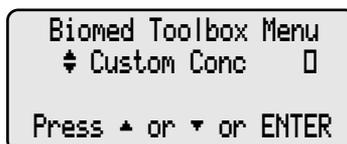

2. To view or customize concentrations, press **ENTER**.
3. Press **▲** or **▼** to select the units (milligrams or micrograms) per ml you wish to customize, then press **ENTER**.

```

Select Units
  ⚡ Milligrams  0
Press ▲ or ▼ or ENTER
  
```

If an X appears in the box, concentrations for these units have been customized.

4. Press **▲** or **▼** to select one of the following, then press **ENTER**.
 - **Turn On All** (this will turn on all concentrations).
 - **Turn Off All** (this will turn off all concentrations except the currently programmed concentration).
 - **Modify Individual** (this allows you to selectively turn on or turn off concentrations).

```

Select
  ⚡ Modify Individual
Press ▲ or ▼ or ENTER
  
```

5. Turn individual concentrations on or off as appropriate:
 - Press **▲** or **▼** to select the concentration.
 - Press **ENTER** to turn the concentration on or off.
 - Repeat as necessary. When finished, press **NEXT** to return to the Biomed Toolbox screen.

```

Select Concentration
  ⚡ 2.0 mg/ml Off
ENTER to turn on
  
```

NOTE: If you try to exit with all concentrations turned off, a message will appear reminding you that at least one concentration must be turned on.

Extended History On/Off (PCA Only)

This screen allows you to turn the Extended History feature on or off. When turned off, Extended History will not appear in Options and the New Patient Marker screen will not appear during programming.

1. At the Biomed Toolbox Menu, press **▲** or **▼** until “Extended History” appears. If an X appears in the box, the Extended History is currently on.
2. To change the setting, press **ENTER**. Press **▲** or **▼** to select the desired setting, then press **ENTER**.

```
Biomed Toolbox Menu
┆ Extended History X
Press ▲ or ▼ or ENTER
```

```
Extended History
┆ On
Press ▲ or ▼ or ENTER
```

Max Doses Per Hour On/Off (PCA Only)

This screen allows you to turn on or turn off Max Doses Per Hour. If the Max Doses Per Hour function is off, doses will not be limited per hour. Doses will be limited only by Demand Dose Lockout Time. When Max Doses Per Hour is changed, any Dose Lockout Time will be cleared. The Event Log will note that the Max Doses Per Hour function was turned on or off.

1. At the Biomed Toolbox Menu, press **▲** or **▼** until “Max Dose Per Hour” appears. If an X appears in the box (X), Max Doses Per Hour function is currently on.
2. To change the setting, press **ENTER**. Press **▲** or **▼** to select the desired setting, then press **ENTER**.

```
Biomed Toolbox Menu
┆ Max Dose Per Hour X
Press ▲ or ▼ or ENTER
```

```
Max Doses Per Hour
┆ On
Press ▲ or ▼ or ENTER
```

PM (Preventive Maintenance) Reminder

If your institution or other health care facility establishes a maintenance program for the pump, you can use the PM Reminder to display a “Prev. Maint. Reminder” message upon power up at a specified interval (1 to 24 months). Once the message begins appearing, it will appear during every power up until it is reset. Use this screen to specify the interval at which the message should appear, or use it to reset the reminder.

- At the Biomed Toolbox Menu, press **▲** or **▼** until “PM Reminder” appears. If an X appears in the box, a PM Reminder is set.
- Press **ENTER**. The PM Reminder screen will appear.
 - Press **ENTER** to reset the reminder, or
 - Press **▲** or **▼** to select the new interval. (To turn the reminder off, select Not In Use.) Then press **ENTER**.
- The date corresponding to your selection (current date + number of months selected) will appear on the screen.

```
Biomed Toolbox Menu
┆ PM Reminder  0
Press ▲ or ▼ or ENTER
```

```
PM Reminder
┆ 2 months
PM Due Date 07/06/00
```

```
Next PM Reminder
  09/06/00
<Entering...>
```

Custom Lock Level Code

This screen allows you to select a new Lock Level Code. Changing this code also changes the Biomed Toolbox Code to **** omitted****. It *does not* affect the Clinician Bolus Code.

- At the Biomed Toolbox Menu, press **▲** or **▼** until “Custom Lock” appears. If an X appears in the box, a Custom Lock Level Code is currently set.

```
Biomed Toolbox Menu
┆ Custom Lock  0
Press ▲ or ▼ or ENTER
```

- To view or change the Custom Lock Level Code, press **ENTER**. The current code will appear.

Custom Lock Code
 ⚡ ***
 <Range: 1 - 899>

- To change the Custom Lock Level Code, press **▲** or **▼** to select the desired code (001 to 899). Then press **ENTER**.

Change Lock Code to
 ***?
 Press Y or N

- Press **▲** to confirm the change.

Date Format

This screen allows you to select the date format. The date can be set to display in US Standard format (*month/day/year*) or in European Standard format (*day/month/year*).

- At the Biomed Toolbox Menu, press **▲** or **▼** until “Date Format” appears. Press **ENTER**.

Date Format
 ⚡ European Standard
 Press ▲ or ▼ or ENTER

- The current format will appear. To change the format, press **▲** or **▼**. Then press **ENTER**.

Change Date Format to
 European Standard?
 Press Y or N

- Press **▲** to confirm the change.

Biomed Toolbox Menu
 ⚡ Date Format
 Press ▲ or ▼ or ENTER

Power Source Status Display

This feature is used to select the power source display on the main screen. You may choose “Always” so the main screen will always indicate the type of power source being used, or “Only Low Battery” to display a message only when the 9 volt battery is low.

1. At the Biomed Toolbox Menu, press **▲** or **▼** until “Power Source” appears. If an X appears in the box, Power Source display is currently set to Always.
2. To change the setting, press **ENTER**. Press **▲** or **▼** to select the desired setting, then press **ENTER**.

```
Biomed Toolbox Menu
  ⚡ Power Source 0
Press ▲ or ▼ or ENTER
```

```
Power Source Display
  ⚡ Always
Press ▲ or ▼ or ENTER
```

Upstream Sensor On/Off (Model 6101 only)

The Upstream Occlusion Sensor screen can be set to on or off. If this screen is set to on, and an upstream occlusion (between pump and fluid container) is detected, an alarm will sound, delivery will stop, and the display will show “Upstream Occlusion.”

WARNING: When the Upstream Occlusion Sensor is turned off, the pump will not detect occlusions upstream (between the pump and fluid container). It is recommended that you periodically inspect the fluid path for kinks, a closed clamp, or other upstream obstructions. Upstream occlusions may result in under- or non-delivery of medications. If undetected, the occlusions could lead to death or serious injury to the patient.

1. At the Biomed Toolbox Menu, press **▲** or **▼** until “Upstream Sensor” appears. If an X appears in the box, the upstream sensor is currently On.
2. To change the setting, press **ENTER**. Press **▲** or **▼** to select the desired setting, then press **ENTER**.

```
Biomed Toolbox Menu
  ⚡ Upstream Sensor 0
Press ▲ or ▼ or ENTER
```

```
Upstream Sensor
  ⚡ On
Press ▲ or ▼ or ENTER
```

3. Press **Y** to confirm the change.

```
Change Upstream
Sensor to On?
```

```
Press Y or N
```

Air Detector Requirement

The Air Detector screen can be set to “Required” or “Not Required.” If this screen is set to “Required,” an Air Detector must be installed and active in order to start the pump; however, the pump may be programmed without an Air Detector.

WARNING: When the Air Detector is not installed, or is installed but turned off, the pump will not detect air in the fluid path. It is recommended that you periodically inspect the fluid path and remove any air to prevent air embolism. Air embolism could result in death or serious injury to the patient.

1. At the Biomed Toolbox Menu, press **Y** or **N** until “Air Detector Req” appears. If an X appears in the box, the Air Detector is currently required.
2. To change the setting, press **ENTER**. Press **Y** or **N** to select the desired setting, then press **ENTER**.
3. Press **Y** to confirm the change.

```
Biomed Toolbox Menu
✦ Air Detector Req 0
Press ▲ or ▼ or ENTER
```

```
Air Detector
✦ Required
Press ▲ or ▼ or ENTER
```

```
Change Air Detector to
Required?
Press Y or N
```

Section 6: Reference & Troubleshooting

Troubleshooting

A continuous two-tone alarm is sounding; the amber light is lit or flashing.

Delivery has stopped. Read the message on the display and refer to the list of messages beginning on the next page. Press **(?)** to see if further information is available. If the display is blank or contains random characters, the 9 volt battery may be depleted; install a new battery. (No help is available during an error or if the battery is depleted.)

The pump is sounding 2 beeps every two seconds; the amber light is flashing.

Look at the message on the display and refer to the list of messages beginning on the next page. Or press **(?)** for further information.

Three beeps sound every 5 minutes.

This is a reminder that the pump is stopped.

After installing a battery, no screen appears and no beep sounds

The battery may have been installed backwards. Review the procedure for installing a battery. Be sure to match the polarity (+ and -) markings on the side of the pump with the markings on the battery. If there is still no power, the battery may be completely depleted.

Lock Level Code does not work, or you forgot the custom code

If the Lock Level Code does not work, it may have been customized (<Custom> will appear on the Lock Level Code screen). If necessary, contact Deltec's Customer Service Department for instructions on reverting to the standard Lock Level Code. If you are trying to use the custom code, it is possible that the Lock Level Code has been reset. If <Custom> does not appear on the Lock Level Code screen, try the standard code.

Printing Problems

Make sure:

- the Interface Cable is connected properly to the Data In/Out jack
- printer switches are set properly (See Instructions for Use supplied with Interface Cable)
- the printer is plugged in and on-line
- paper is loaded with the correct side facing out, and paper is not jammed

Refer also to the printer manual supplied with the printer.

An Air In Line alarm keeps occurring even though the Air Detector was turned off

Any time you power up the pump in Lock Level 0, the Air Detector will automatically turn on. In other words, the pump will automatically change the Air Detector Option setting from “Turned Off” to “Turned On.” (This does not occur in Lock Level 1 or 2.) If you do not want to use the Air Detector, you will need to change the Air Detector Option setting back to “Turned off” after the pump powers up. If the Lock Level is LL1 or LL2 when the pump powers up, the Air Detector Option setting will remain “Turned Off.”

Unable to view Extended History (PCA)

Extended History is turned off in the Biomed Toolbox. If appropriate, turn Extended History on (Section 5).

Unable to select Micrograms (PCA)

Micrograms are turned off in the Biomed Toolbox. If appropriate, turn on Micrograms (Section 5).

Unable to add a New Patient Marker during programming (PCA)

Extended History is turned off in the Biomed Toolbox. If appropriate, turn Extended History on (Section 5).

Unable to select a specific concentration (PCA)

The concentration may be turned off in the Biomed Toolbox. If appropriate, turn the concentration on (Section 5). Or, the concentration may not be programmable (see scroll range tables, this section).

Alarms and Messages, Alphabetical List

Message	Corrective Action
9 volt Battery Depleted / Install good battery	Install a new 9 volt battery. The pump will not start with a depleted 9 volt battery. A good battery must always be installed even when an external source of power is connected. NOTE: This message may appear when you install a new battery while an external source of power is connected. Remove and reinstall the battery to cancel this message, then restart the pump if necessary.
9 volt Battery Low	The 9 volt battery is low but the pump is operable. Change the 9 volt battery soon. NOTE: This message may appear when you install a new battery while an external source of power is connected. Remove and reinstall the battery to cancel this message.
9 volt Battery Removed / Install good battery	The 9 volt battery has been removed with an external power source attached. Install a new 9 volt battery. Install a battery within 3 minutes to keep the pump running; after 3 minutes, the pump will stop.
9 volt Battery Removed / Pump will not run	The 9 volt battery was removed with an external power source attached. The pump is stopped. Press  to silence the alarm, then install a new battery.
AC Adapter Disconnected	The AC Adapter has been disconnected and the pump is being powered by the 9 volt battery. If desired, reconnect the AC Adapter.
AC Adapter Unpowered / Check power source	The AC Adapter is not receiving power from the wall outlet. The 9 volt battery is supplying power. Make sure the AC Adapter is properly plugged into the wall outlet and the wall outlet is supplying power. If the alarm persists, the AC Adapter may be faulty and may need to be replaced.
Air Detector Port Cover Removed / Install Cover	The cover for the Air Detector port on the side of the pump must be properly attached for the pump to operate. Remove all power. Make sure the cover is installed properly, then resume operation.

Message	Corrective Action
Air Detector Fault / Pump will not run	The Air Detector is faulty. Press (NEXT) to silence the alarm. Close the tubing clamp, remove the pump from use, and replace the Air Detector.
Air Detector Removed?	The Air Detector has been removed. If this is acceptable, press ▲ . If the Air Detector <i>should</i> be installed or has not actually been removed, press ▼ . Then have an Air Detector installed properly. If an Air Detector is attached and the alarm persists, have the Air Detector serviced.
Air Detector Required / Pump will not run	This message indicates that an Air Detector is required to start the pump (i.e. the Air Detector setting in the Biomed Toolbox is “Required”). If necessary, press (NEXT) to silence the alarm, then have an Air Detector installed.
Air in line detected / Pump will not run	The Air Detector has detected air in the fluid path; the fluid path may contain air bubbles, or the tubing may not be threaded through the Air Detector. Press (NEXT) to silence the alarm, then: <ul style="list-style-type: none"> • Make sure the tubing is threaded properly. • If the fluid path contains air bubbles, close the clamps and disconnect the fluid path from the patient. Then follow the instructions for removing air using the Prime Option in Section 4.
All Concentrations cannot be turned off	PCA: At least one concentration must be enabled when customizing concentrations. Press (NEXT) , then enable a concentration.
Cable Removed	The cable was detached from the Data In/Out jack.
Cassette Damaged / Free flow may occur / Clamp Tubing / Change Cassette	The pump detects the cassette is damaged. Close the tubing clamp and inspect the cassette for damage. Replace it if necessary.
Cassette Not Attached / Pump will not run	The pump will not start without a cassette attached. Make sure a cassette is attached properly. Then start the pump.

Message	Corrective Action
Cassette Unlocked	PCA: The PCA delivery mode requires the cassette to be locked onto the pump before it can be started. If an alarm is sounding, press ◻NEXT to silence the alarm. Lock the cassette, then start the pump.
Cassette Unlatched / Close clamp to prevent free flow	This message appears as a reminder to close the tubing clamp when the cassette is unlatched from the pump.
Change (setting) to (X)?	The message is asking for confirmation of the value you entered. If it is correct, press ▲ . If it is incorrect, press ▼ and choose the correct value. If this message appears when you try to use ◻NEXT to go to the next screen, you may have changed a setting that requires you to verify the setting shown on this screen or to program a new setting.
Changing Modes clears program and Event Log	When you select a delivery mode, even if you select the current mode, the Event Log clears and the program is set to the default settings. Press ▲ if you wish to continue, or press ▼ to return to the Change Mode screen.
Changing the date (or time) may affect the next dose start time. Review before delivery.	INTERMT: When the date or time is changed, the next dose start time is adjusted. Review the next dose start time before starting delivery.
Changing time will clear Extended History and reset dose lockout time	PCA: When the time is changed, the Extended History is cleared. The Lockout time is also reset so a Demand Dose can be requested immediately.
Check for empty tubing or reservoir	The tubing beneath the pump may not contain fluid, or the fluid container may be empty. Check whether the fluid container is empty; or clamp the tubing, remove the cassette, and check for air in the tubing. If the alarm persists after trying to correct the problem, remove the pump from use and contact Customer Service.

Message

Corrective Action

Clinician Bolus not available during Demand Dose

PCA: A Clinician Bolus may not be started while a Demand Dose is being delivered. Wait until the Demand Dose finishes, then start the Clinician Bolus if appropriate.

Clock Battery needs service soon

The clock battery must be replaced soon. When feasible, remove the pump from use and return it for replacement of the clock battery.

Clock Battery is low / Service immediately

The clock battery is low and must be serviced. Close the tubing clamp and remove the pump from use. Contact Customer Service for replacement of the clock battery.

Communications Failed

The pump is on the receiving end of Communications, and Communications has failed. Press **NEXT** to silence the alarm. Wait for the person initiating communications to call you back. Make sure your modem phone is hung up.

Current Concentration cannot be turned off

PCA: The currently programmed Concentration cannot be disabled. Exit the Biomed Toolbox and change to a different Concentration. Then return to the Biomed Toolbox and turn off this concentration.

Delivery Stopped (Model 6101 only)

Fluid is not flowing from the fluid container to the pump. Check for a kink, a closed clamp, or an air bubble in the tubing between fluid container and pump. Press **STOP START** to stop the pump and silence the alarm for 2 minutes, then remove the obstruction and press **NEXT** to restart the pump.

Delivery Too Slow / External power source must be connected

The 9 volt battery does not provide sufficient power to support the programmed delivery rate. Connect an external source of power. Or, if appropriate, acknowledge the message and allow delivery to proceed at the lower rate by pressing **NEXT**.

Message	Corrective Action
Dose Duration is being lengthened	INTERMT: You have entered a new volume that would cause the delivery rate to exceed the maximum rate of 350 ml/hr. The pump has automatically lengthened the Dose Duration to accommodate the volume you entered, but you will need to either confirm that this new duration is acceptable or enter a new duration.
Dose Cycle is being lengthened	INTERMT: The Dose Duration you entered exceeds the Dose Cycle that is currently programmed. The pump has automatically lengthened the Dose Cycle, but you will need to either confirm that the new cycle is acceptable or enter a new cycle.
Dose Not Delivered / Dose not available when pump is stopped	PCA: The pump must be running in order to start a Demand Dose. First start the pump, then request a Demand Dose.
Dose Not Delivered / Dose Locked Out	PCA: The Lockout Time or Max Doses per Hour is preventing the Demand Dose from being delivered. Wait until the lockout time elapses before requesting a Demand Dose.
Dose Not Delivered / No Dose programmed	PCA: The Demand Dose amount is set to 0. Therefore, a Demand Dose cannot be delivered.
Dose scheduled to start in — minutes / Start the pump	INTERMT: The pump is stopped, but a dose is scheduled to be delivered in the number of minutes indicated. In order for the dose to be delivered, you must start the pump.
Dose scheduled to start is now overdue / Start the pump	INTERMT: The pump is stopped, but a dose is overdue for its scheduled delivery. In order for the dose to be delivered, you must start the pump.
Error Detected / E (<i>code</i>)	A pump fault has occurred. Close the tubing clamp and remove the pump from use. Contact Customer Service to return the pump for service.

Message	Corrective Action
External Power Needed for High Rate	An external power source must be attached to achieve the rate that has been programmed.
External Power Source Faulty / Change Power Source	The power pack or the AC Adapter is faulty. Ensure the cords and cables are properly attached. If this does not correct the problem, replace the power source.
High Pressure	The pump has detected high pressure, which may be resulting from a downstream blockage, kink in the fluid path, or a closed tubing clamp. Remove the obstruction to resume operation. Or, press STOP START to stop the pump and silence the alarm for 2 minutes, then remove the obstruction and restart the pump.
High Volume Admin set not supported in this version of PCA / Remove admin set	The CADD-Prizm® High Volume Administration Set cannot be used with the PCA delivery mode. You must remove the set to continue.
High Volume Admin set Required	A CADD-Prizm® High Volume Administration Set is required to deliver the programmed rate. Remove the current cassette and replace with a CADD-Prizm® High Volume Administration Set.
Infusion Period is being lengthened	TPN: The new setting you entered would cause the Plateau Rate to exceed the maximum of 350 ml/hr. The Infusion Period has been lengthened to accommodate the new setting. Press NEXT , then confirm the new Period or program a different Period.
Infusion Period is being shortened	TPN: The new setting you entered would cause the Plateau Rate to be less than the minimum of 10 ml/hr. The Infusion Period has been shortened to accommodate the new setting. Press NEXT , then confirm the new Period or program a different Period.
Insufficient External Power	The AC Adapter is not receiving power or the power pack is completely depleted. Ensure the cords and cables are properly attached. Or, begin recharging the power pack.

Message	Corrective Action
Key Stuck / Release key or remove power to stop pump	A key may be pressed down. Make sure there is nothing pressing on any of the keys. If the alarm persists, close the tubing clamp and remove the pump from use. Contact Customer Service to return the pump for service.
Lock cassette before starting	PCA: The cassette has been properly latched. Lock the cassette or the pump will not run.
Micrograms On / Cannot turn off current programming units	PCA: Micrograms cannot be turned off because they are the current programming units. First, change the Units, then turn off Micrograms.
Motor is temporarily disabled / Remove power and restart pump	The pumping mechanism temporarily stopped. Remove the external power source (if applicable). Then remove and reinsert the 9 volt battery and reconnect the external power source if desired. Restart the pump.
Motor service due	The pump's motor requires service. Remove the pump from use at the next cassette change and contact Customer Service to return the pump for service.
No Air Detector attached	This message appears at power up to inform you that no Air Detector is attached to the pump. "Air Eliminating Filter Recommended" will also appear if the pump is in the TPN delivery mode.
No changes allowed	The current lock level does not allow changes to the setting displayed on the screen.
No Dose Volume Programmed / Pump will not run	INTERMT: The pump will not start if a dose has not been programmed. Follow the instructions in Section 2 for programming the pump.
No Rate or Dose Programmed / Pump will not run	PCA: The pump will not start if no rate or doses have been programmed. Follow the instructions in Section 2 for programming the pump.
Possible hardware problem / Service pump	There may be a hardware problem with the Air Detector. Have the Air Detector replaced.

Message

Corrective Action

Power Pack Depleted /
Change Power Source

The power pack is depleted and unable to support pump operation. The 9 volt battery is supplying power. Recharge the power pack with the AC Adapter.

Power Pack Disconnected

The power pack is disconnected from the pump. Reconnect the power pack, attach an AC Adapter, or allow the pump to run on the 9 volt battery power.

Prev. Maint. Reminder (date)

Your institution may have established a maintenance program for the pump and preventive maintenance is due. Refer to your institution's policy.

Print Failure /
Check printer & cable

Printing has stopped. The paper may be out or jammed, the printer may have lost power, or the printer may be off-line. Press **(NEXT)** to silence the alarm and refer to the printer manual to correct the problem. Then remove and reattach the cable and repeat printing.

Printing Stopped /
Print Again?

During printing, **▼** was pressed, signalling printing to stop. To start over, press **▲**. To exit printing, press **▼**.

Range: Limited

This message appears on rate, dose, or Reservoir Volume screens when the pump is in LL1. It indicates that the range of programmable values is limited by the value programmed in LL0 (i.e. you cannot increase the value beyond what was programmed in LL0).

Reservoir Volume is zero

The Reservoir Volume has reached 0.0 ml. Press **(NEXT)** to stop the alarm. Then install a new fluid container if appropriate.

Reservoir Volume Low

The Reservoir Volume value is low, indicating that the level of fluid in the fluid container is low. Prepare to install a new fluid container.

Reset Reservoir Volume to
(X) ml?

If you wish to reset the Reservoir Volume to the originally programmed value, press **▲**. To leave the Reservoir Volume value unchanged, press **▼**.

Message**Corrective Action**

To continue, unlatch and remove the Admin set or reservoir / Then reattach

The cassette was not completely removed from the pump before it was reattached and, therefore, the pump's sensors are not able to detect the cassette type. Remove the cassette and reattach it, then verify the cassette type in the pump's display. If this alarm persists, remove the pump from use and contact Customer Service to return the pump for service.

Upstream Occlusion /
Press STOP to silence
(Model 6101 only)

Fluid is not flowing from the fluid container to the pump. Check for a kink, a closed clamp, or air bubbles in the tubing between fluid container and pump. Press  to stop the pump and silence the alarm for 2 minutes, then remove the obstruction and press  to restart the pump.

Upstream Occlusion /
Press STOP to silence /
Press NEXT to restart
(Model 6101 only)

Fluid is not flowing from the fluid container to the pump. Check for a kink, a closed clamp, or air bubbles in the tubing between fluid container and pump. Press  to stop the pump and silence the alarm, then remove the obstruction and press  to restart the pump.

Wrong Cassette

The pump detects the cassette is damaged, attached improperly, or incompatible with the pump. Close the tubing clamp. Make sure the cassette is attached properly. Then open the clamp and restart the pump. If the alarm persists, you may need to replace the cassette.

Cleaning the Pump and Accessories

CAUTION:

- Do not immerse the pump in cleaning fluid or water. Do not allow solution to soak into the pump, accumulate on the keypad, or enter the battery compartment, Data In-Out jack, Power jack or Air Detector Port area. Moisture buildup inside the pump may damage the pump.
 - Do not clean the pump with acetone, other plastic solvents, or abrasive cleaners, as damage to the pump may occur.
-

Use any of the following solutions to clean the pump and accessories:

- Soap solution
 - Benzalkonium Chloride concentrate (0.13%)
 - Glutaral Concentrate, USP (2%)
 - 10 percent solution of household bleach (one part household bleach to nine parts water)
 - Alcohol, USP (93%)
 - Isopropyl Alcohol, USP (99%)
1. Dampen a soft, lint-free cloth with cleaning solution. Apply the solution to exterior surface of the pump or accessory. *Do not allow the solution to soak into the pump or accessory.*
 2. Wipe the entire surface dry with another soft, lint-free cloth. Allow the pump to dry completely before use.

Cleaning the Battery Contacts

Routinely clean the battery contacts, possibly as part of the preventative maintenance cycle, to remove buildup of foreign material on the contacts.

Use the following to clean the contacts:

- Cotton swab wetted with Isopropyl Alcohol (70% minimum)

NOTE: Do not use an alcohol formulation that contains components other than alcohol and water.

OR

- Pre-moistened alcohol swab
1. Using a swab wetted with alcohol, rub the entire battery contact for a minimum of ten back and forth cycles (twenty total wipes over the contact).
 2. Using a clean surface of the swab, repeat the process for the second battery contact.
 3. Using a clean swab wetted with alcohol, rub each battery contact again, a minimum of four back and forth cycles (eight total wipes over the contact).
 4. Allow the contacts to dry completely before use.

Exposure to Radiation or Magnetic Resonance Imaging (MRI)

CAUTION:

- Do not expose the pump to therapeutic levels of ionizing radiation as permanent damage to the pump's electronic circuitry may occur. The best procedure to follow is to remove the pump from the patient during therapeutic radiation sessions. If the pump must remain in the vicinity during a therapy session, it should be shielded, and its ability to function properly should be confirmed following treatment.
 - Do not expose the pump directly to ultrasound, as permanent damage to the pump's electronic circuitry may occur.
 - Do not use the pump in the vicinity of magnetic resonance imaging (MRI) equipment as magnetic fields may adversely affect the operation of the pump. Remove the pump from the patient during MRI procedures and keep it a safe distance away from magnetic energy.
 - Do not use the pump near ECG equipment as the pump may interfere with the operation of the equipment. Monitor ECG equipment carefully when using this pump.
-

PCA Delivery Mode: Continuous Rate Scroll Ranges

Units	Starting Value	Increment	Maximum	
Milliliters	0.10	0.10	30.00	
Milligrams & Micrograms	10% of concentration	Mg only: Values between 0.01 and 0.5: Mcg only: Values between 0.1 and 0.5: Values between 0.5 and 100: Values between 100 and 1000: Values greater than 1000:	0.01 0.1 0.1 1.0 10.0	Concentration × 30

PCA Delivery Mode: Demand Dose, Clinician Bolus Scroll Ranges, Milliliters

Milliliters			
Demand Dose		Clinician Bolus	
increment	max.	increment	max.
0.05	9.9	0.05	20

PCA Delivery Mode: Demand Dose, Clinician Bolus Scroll Ranges, Milligrams

Concentration mg/ml	Milligrams			
	Demand Dose increment	max.	Clinician Bolus increment	max.
0.1	0.01	0.99	0.01	2
0.2	0.02	1.98	0.02	4
0.3	0.03	2.97	0.03	6
0.4	0.04	3.96	0.04	8
0.5	0.05	4.95	0.05	10
1	0.05	9.9	0.05	20
2	0.10	19.8	0.10	40
3	0.15	29.7	0.15	60
4	0.20	39.6	0.20	80
5	0.25	49.5	0.25	100
10	0.50	99.0	0.50	200
15	0.75	148.5	0.75	300
20	1.00	198.0	1.00	400
25	1.25	247.5	1.25	500
30	1.50	297.0	1.50	600
35	1.75	346.5	1.75	700
40	2.00	396.0	2.00	800
45	2.25	445.5	2.25	900
50	2.50	495.0	2.50	1000
55	2.75	544.5	2.75	1100
60	3.00	594.0	3.00	1200
65	3.25	643.5	3.25	1300
70	3.50	693.0	3.50	1400
75	3.75	742.5	3.75	1500
80	4.00	792.0	4.00	1600
85	4.25	841.5	4.25	1700
90	4.50	891.0	4.50	1800
95	4.75	940.5	4.75	1900
100	5.00	990.0	5.00	2000

PCA Delivery Mode: Demand Dose, Clinician Bolus Scroll Ranges, Micrograms

Concentration mcg/ml	Micrograms			
	Demand Dose increment	max.	Clinician Bolus increment	max.
1	0.05	9.9	0.05	20
2	0.10	19.8	0.10	40
3	0.15	29.7	0.15	60
4	0.20	39.6	0.20	80
5	0.25	49.5	0.25	100
10	0.50	99.0	0.50	200
15	0.75	148.5	0.75	300
20	1.00	198.0	1.00	400
25	1.25	247.5	1.25	500
30	1.50	297.0	1.50	600
35	1.75	346.5	1.75	700
40	2.00	396.0	2.00	800
45	2.25	445.5	2.25	900
50	2.50	495.0	2.50	1000
55	2.75	544.5	2.75	1100
60	3.00	594.0	3.00	1200
65	3.25	643.5	3.25	1300
70	3.50	693.0	3.50	1400
75	3.75	742.5	3.75	1500
80	4.00	792.0	4.00	1600
85	4.25	841.5	4.25	1700
90	4.50	891.0	4.50	1800
95	4.75	940.5	4.75	1900
100	5.00	990.0	5.00	2000
200	10.00	1980.0	10.00	4000
300	15.00	2970.0	15.00	6000
400	20.00	3960.0	20.00	8000
500	25.00	4950.0	25.00	10000

Military Time Conversion Chart

12-Hour Time	Military Time
12:00 AM (midnight)	00:00
1:00 AM	01:00
2:00 AM	02:00
3:00 AM	03:00
4:00 AM	04:00
5:00 AM	05:00
6:00 AM	06:00
7:00 AM	07:00
8:00 AM	08:00
9:00 AM	09:00
10:00 AM	10:00
11:00 AM	11:00
12:00 PM (noon)	12:00
1:00 PM	13:00
2:00 PM	14:00
3:00 PM	15:00
4:00 PM	16:00
5:00 PM	17:00
6:00 PM	18:00
7:00 PM	19:00
8:00 PM	20:00
9:00 PM	21:00
10:00 PM	22:00
11:00 PM	23:00

Specifications (Nominal)

General Pump Specifications

Resolution	Medication Cassette™ Reservoir or CADD® Administration Set, 0.050 ml/pump stroke nominal CADD-Prizm® High Volume Administration Set, 0.100 ml/pump stroke nominal
Size	4.4 cm × 10.4 cm × 14.1 cm (1.7 in. × 4.1 in. × 5.6 in.) excluding cassette or other accessories
Weight	568 g (20 oz.) including 9 volt battery and empty 100 ml Medication Cassette™ Reservoir, excluding other accessories
Pump Alarms	Low battery power; depleted battery power; external power source low, faulty, depleted; pump stopped; pump fault; low reservoir volume; high delivery pressure; air in line; Air Detector faulty or detached (only with the use of the optional Air Detector); Air Detector Port Cover detached; delivery too slow; key stuck; cassette detached or unlocked; print failure.
Bolus Volume at Occlusion	
Alarm Pressure	0.050 ml resolution administration sets/Medication Cassette™ Reservoirs: <0.25 ml 0.100 ml resolution administration sets: <2.0 ml
Power Sources	9 volt alkaline or lithium battery such as DURACELL® Alkaline MN 1604 or ULTRALIFE® Lithium U9VL; CADD® External Power Source (EPS) Power Pack reorder number 21-3801; AC Adapter.

The expected life of a 9 volt battery is 12 hours at 100 ml/hour, or approximately 5 days at 10 ml/day (nominal). This estimate is based on laboratory tests conducted at room temperature using a new battery. Actual battery life will vary depending on the brand of battery, battery shelf life, temperature conditions, delivery rate, and frequency of screen display, back-lighting and printing. It is recommended that a new 9 volt battery be kept available for replacement if necessary.

An internal battery powers the clock. When it is depleted, it cannot reliably maintain the clock time. This battery must be replaced by the manufacturer. The internal battery has an expected life of 5 years.

System Operating	
Temperature	+2°C to 40°C (36°F to 104°F)
System Storage Temperature	-20°C to 60°C (-4°F to 140°F)
Power Pack Charging	
Temperature	+10°C to 35°C (50°F to 95°F)
System Delivery Accuracy	± 6% (nominal)
System Definition	System is defined as a CADD-Prizm® pump with an attached Medication Cassette™ Reservoir and CADD® Extension Set with integral anti-siphon valve, or an attached CADD® Administration Set with integral or add-on anti-siphon valve.
High Pressure Alarm	18 ± 9 psi [2.76 bar]
Air Detector Alarm	Single bubble greater than 0.100 ml

PCA Delivery Mode Specifications

Reservoir Volume	1 to 9999 or Not In Use; programmable in 1 ml increments, displayed in 0.1 ml increments Default: 1 ml
Units	Milliliters (ml), milligrams (mg), micrograms (mcg) Default: milligrams
Concentration	Mg/ml: 0.1, 0.2, 0.3, 0.4, 0.5, 1, 2, 3, 4, 5, 10, 15, ... 95, 100 Mcg/ml: 1, 2, 3, 4, 5, 10, 15, ...95, 100, 200, 300, 400, 500 Default: 1
Continuous Rate	0 – 30 ml/hr (or the mg or mcg equivalent) Default: 0 mg/hr
Demand Dose	0 to 9.9 ml Default: 0 mg/hr Delivery rate (Continuous Rate + Demand Dose): 125 ml/hr nominal

Demand Dose Lockout	5 minutes to 24 hours in the following increments: 1 minute for values between 5 and 20 minutes 5 minutes between 20 minutes and 24 hours Default: 5 minutes
Max Doses Per Hour	1 – 12 doses in 1 dose increments (will also be limited by the Demand Dose Lockout value) Default: 1
Demand Doses Given.....	0 to 999
Demand Dose Attempts	0 to 999
Given	0 to 99999.99 in 0.01 unit increments
Clinician Bolus	0.1 ml to 20.00 ml (or mg or mcg equivalent) Delivery rate (Continuous Rate + Clinician Bolus): 125 ml/hr nominal

Continuous Delivery Mode Specifications

Reservoir Volume	1 to 9999 or Not In Use; programmable in 1 ml increments, displayed in 0.1 ml increments Default: 1 ml
Continuous Rate	0.1 – 350 ml/hr in the following increments: 0.1 for values between 0.1 and 100 1 for values between 100 and 350 Default: 0 ml/hr Use 9 volt battery for rates up to 250 ml/hr; use power pack or AC adapter for rates up to 350 ml/hr.
Given	0 to 99999.9 in 0.1 unit increments

TPN Delivery Mode Specifications

Reservoir Volume	10.0 to 9990 or Not In Use; programmable in 1 ml increments, displayed in 0.1 ml increments Default: 10 ml
Infusion Volume	10 – 9990 ml in 10 ml increments: Default: 10 ml
Infusion Period	0 hrs 10 min - 99 hrs 50 min in 10 minute increments: Default: 1 hr 0 min
Taper-Up Period	0 hrs 0 min - 99 hrs 40 min in 10 minute increments: Default: 0 hrs 0 min

Taper-Down Period	0 hrs 0 min - 99 hrs 40 min in 10 minute increments: Default: 0 hrs 0 min
Plateau Rate	Calculated by pump; 10 - 350 ml/hr Use 9 volt battery for rates up to 250 ml/hr; use power pack or AC adapter for rates up to 350 ml/hr.
KVO Rate	Calculated by pump: $\frac{1}{10}$ of Plateau Rate up to 5 ml/hr
Given	0 to 99999 in 0.1 unit increments

Intermittent Delivery Mode Specifications

Reservoir Volume	1 to 9999 or Not In Use; programmable in 1 ml increments, displayed in 0.1 ml increments Default: 1 ml
Dose Volume	0.1 – 1000 ml in the following increments: 0.1 for values between 0.0 and 100 1 for values between 100 and 1000 Default: 0.0 ml
Dose Duration	1 min - 24 hrs in the following increments: 1 minute for values between 1 min and 10 min 5 minutes for values above 10 min Default: 30 min Duration is limited by Dose Volume so that rate does not exceed 350 ml/hr. Use 9 volt battery for rates up to 250 ml/hr; use power pack or AC adapter for rates up to 350 ml/hr.
Dose Cycle	10 min - 96 hrs in 5 minute increments: Default: 4 hrs
KVO Rate	0 - 10 ml/hr in 0.1 ml/hr increments Default: 0 ml/hr
Next Dose Start Time	10 min - 96 hrs X min (where X equals a 10-minute increment in the 96th hour) or Immediate; program- mable in 10 minute increments Default: Immediate
Given	0 to 99999.9 in 0.1 unit increments
Time Remaining	Dose and Cycle display in 1 minute increments

Options Specifications

Immediate Taper-Down (TPN) ..	0 to time remaining in the infusion period, in 10 minute increments (defaults to the currently programmed Taper-Down)
AutoLock	Not In Use, LL1, or LL2
Time	00:00 to 23:59
Air Detector	Turned On or Turned Off
Event Log	0 – 500 events
Extended History	Up to 48 hours in 1 hour increments

Biomed Toolbox Specifications

PM (Preventive Maintenance)	
Reminder	1 to 24 months in 1 month increments, Not In Use
Custom Lock Level Code	1 – 899 (excluding preset code) in increments of 1
Date Format	US Standard (mm/dd/yy) or European Standard (dd/mm/yy)
Power Source Display	Always display or Only Low Battery
Air Detector Required	Required or Not Required

Printed Reports

An Interface cable is available for printing or communications. Three types of reports are available: the Rx Settings Report lists the pump's current program; the Event Log Report includes Rx settings and the event log through the last 500 events or the last delivery change mode (see Section 4 for a description of the event log); the Extended History Report lists current pump settings, amount of medication delivered, and hourly dose summaries for the time period you specify (for the past 48 hours or to the last New Patient Marker or Change in Units, Time, or Date; beyond any of these events, the report will show zeroes). Extended History must be on in the Biomed Toolbox for this report to be available.

For additional information on printing or communications, see the *Instructions for Use* provided with the interface cable.

Index

Bold page numbers indicate figure references.

Symbols

“?” key. *See* Help key

A

AC Adapter, 5, 6, 89, 105
 Access Code, 10, 73
 administration
 warning, iv
 administration set, 6, 94
 warning, iv
 Air Detector, 5, 86, 90, 95, 105, 109
 loading tubing into, 62
 status screen, 22, 27, 36, 38, 43, 46, 51, 54
 turning on/off, 77
 Air Detector alarm, 88, 90
 Air Detector Port Cover, 5
 Air Detector Requirement, 77, 86, 90, 109
 alarms, 89-97, 105
 amber indicator light, 3, 4, 65
 Anti-Siphon Valve
 warning, iv
 AutoLock, 10, 11, 65, 109
 setting, 74

B

backlighting, 4
 battery, 9 volt, 3, 6, 9, 85, 89, 105, 106, 109
 installing, 13
 warning, iv
 battery, clock, 75, 92
 battery life, 13, 105

Biomed Toolbox, 19, 22, 71, 79
 Air Detector Requirement, 86, 90
 Concentration Customization, 80
 Custom Lock Level Code, 83
 Date Format, 84
 Extended History on/off, 82
 micrograms on/off, 80
 Power Source Status Display, 85
 Preventive Maintenance Reminder, 83
 screen map, 79
 specifications, 109
 Upstream sensor on/off, 85
 Biomed Toolbox Code, 10, 79, 83
 blood
 warning, iii

C

cassette, 3
 warnings, iv, v
 attaching, 58
 removing, 57
 cassette latch, 6, 58
 cassette lock, 7, 59
 cautions, vi
 Clinician Bolus, 91, 92, 107
 starting, 30
 stopping, 33
 Clinician Bolus Code, 10, 30
 clock battery, 92
 Communications option, 67
 concentration, 90, 92, 106
 programming, 24
 concentrations, customizing, 80-81
 Continuous delivery mode
 main screen, 8
 programming example, 37-38
 programming screens, 34-36
 specifications, 107
 Continuous Rate, 20, 29, 35, 39, 106, 107
 programming, 18, 24, 34, 37
 Custom Lock Level Code, 10, 83, 85, 87, 109

cycle, 48, 55, 70

D

Data In/Out jack, 3, 5
 date, 11, 76
 warning, v
 date format, 84, 109
 DELAY message, 9
 delivery mode, 1, 15
 changing, 11, 73
 Demand Dose, 18, 20, 21, 24, 25, 29, 75,
 93, 106, 107
 programming, 25
 starting, 32
 stopping, 33
 Demand Dose Lockout, 21, 32
 programming, 25
 Dose Counters, 21, 26
 clearing, 26
 Dose Cycle, 50, 53, 93, 108. *See also*
 cycle
 Dose Duration, 50, 53, 93, 108
 Dose key, 20, 32
 Dose Rate, 51, 54
 Dose Volume, 50, 53, 95, 108
 Doses Hour by Hour, 71, 72
 Downstream occlusion sensor, 7

E

epidural administration
 warning, iv
 Event Log, 11, 22, 27, 73, 78, 109
 Event Log Report, 109
 Extended History, 22, 27, 70, 75, 76, 109
 Doses Hour by Hour, 71
 Extended History Report, 109
 Patient Review, 71, 72
 turning on/off, 82
 viewing, 70
 Extension Set, 59
 warning, iv

G

Given screen, 21, 27, 35, 38, 43, 46, 51,
 54, 107, 108
 clearing, 27, 38, 46, 54
 green indicator light, 3, 4, 65

H

Help, help key, 4, 8, 9, 11

I

Immediate Taper-Down, 11, 68, 109
 indicator lights, 3, 4, 65
 Infusion Period, 42, 45, 68, 94, 107
 infusion profile, 40, 42, 47, 60, 68
 Infusion Volume, 42, 45, 107
 Interface Cable, 5
 Intermittent delivery mode, 70
 main screen, 8
 programming example, 52–54
 programming screens, 48–51
 specifications, 108

K

keypad, keys, 3, 4
 KVO rate, 40, 43, 45, 48, 50, 53, 70, 108

L

latch, cassette, 3, 6, 58
 lock, cassette, 3, 7, 59
 lock level, 4, 9, 10, 11, 65
 changing, 63, 65
 Lock Level Code, 10, 16, 63
 customizing, 10, 83
 Lockout, Demand Dose, 21, 25, 32

M

Magnetic Resonance Imaging, 100
main screen, 8, 65, 85
Marker, New Patient, 22, 27
Max Doses Per Hour, 107
 programming, 26
messages, list, 89
micrograms, 19, 80, 82, 88, 95, 106
 turning on/off, 80
military time conversion table, 104

N

“N” (No) key, 5
New Patient Marker, 22, 27
Next Dose Start Time, 48, 51, 53, 55, 70,
 91, 108

O

occlusion sensor, downstream. *See*
 downstream occlusion sensor
occlusion sensor, upstream. *See* upstream
 occlusion sensor
Options, 11, 22, 51, 67–78
 Air Detector On/Off, 77
 Date, 76
 screen map, 67
 specifications, 109
 Time, 75

P

Patient Review, 71, 72
PCA delivery mode
 main screen, 8
 programming example, 23–28
 programming screens, 17
 specifications, 106
Plateau Rate, 43, 45, 94, 108
PM Reminder, 109. *See* Preventive
 Maintenance Reminder
Polemount Bracket, 6

Polemount Bracket recess, 3
Power jack, 3, 5
power pack, 6, 96, 106
Power Source Status display, 8, 85, 109
power-up, 15, 83
Preventive Maintenance Reminder
 setting/resetting, 83
priming, 11, 19, 21, 35, 41, 50, 61, 69
 warning, v
printing, 5, 11, 87, 96, 109
programming
 screen map, 18, 34, 40, 48, 67, 79

R

radiation, exposure to, 100
rate. *See* Continuous Rate
rate display, 43, 45
Remote Dose Cord, 5, 20, 32
reservoir, 6, 19, 35, 41, 50, 96, 97, 105
 warning, iv
Reservoir Volume, 7, 8, 11, 18, 19, 22,
 23, 35, 37, 40, 41, 44, 48, 49, 50,
 52, 53, 61, 66, 96, 105, 106, 107,
 108
resetting, 60, 66

S

security codes
 Access Code, 10
 Biomed Toolbox Code, 10, 79, 83
 Clinician Bolus Code, 10
 customizing, 10, 83
 Lock Level Code, 10, 16, 63, 83, 87
specifications, 105–109
subarachnoid administrations
 warning, iv
syringe
 warning, iii

T

Taper-Down Period, 43, 45, 68, 108
Taper-Up Period, 42, 45, 107
Telecommunications, 67
time, 11, 75, 109
Time Remaining (Intermittent), 11, 70, 108
TPN delivery mode, 68
 main screen, 8
 programming example, 44–46
 programming screens, 40–43
 specifications, 107
 starting infusion, 47
Troubleshooting, 87

U

units, 19, 106. *See also* micrograms
 programming, 24
Upstream occlusion sensor, 7, 58, 85, 92, 97

W

warnings, iii

Y

“Y” (Yes) key, 5

Limited Warranty

SIMS Deltec, Inc. (the “Manufacturer”) warrants to the Original Purchaser that the infusion pump (the “Pump”), not including accessories, shall be free from defects in materials and workmanship under normal use, if used in accordance with this Operator’s Manual, for a period of two years from the actual date of sale to the Original Purchaser. **THERE ARE NO OTHER WARRANTIES.**

This warranty does not cover normal wear and tear and maintenance items, and specifically excludes batteries, administration sets, extension sets or any other accessory items or equipment used with the Pump.

Subject to the conditions of and upon compliance with this Limited Warranty, the Manufacturer will repair or replace at its option without charge (except for a minimal charge for postage and handling) any Pump (not including accessories) which is defective if a claim is made during such two-year period.

The following conditions, procedures, and limitations apply to the Manufacturer’s obligation under this warranty:

A. Parties Covered by this Warranty: This warranty extends only to the Original Purchaser of the Pump. This warranty does not extend to subsequent purchasers. The Original Purchaser may be a patient, medical personnel, a hospital, or institution which purchases the Pump for treatment of patients. The Original Purchaser should retain the invoice or sales receipt as proof as to the actual date of purchase.

B. Warranty Performance Procedure: Notice of the claimed defect must be made in writing or by telephone to the Manufacturer as follows: Customer Service Department, SIMS Deltec, Inc., 1265 Grey Fox Road, St. Paul, MN 55112, (800) 426-2448. Notice to the Manufacturer must include date of purchase, model and serial number, and a description of the claimed defect in sufficient detail to allow the Manufacturer to determine and facilitate any repairs which may be necessary. **AUTHORIZATION MUST BE OBTAINED PRIOR TO RETURNING THE PUMP.** If authorized, the Pump must be properly and carefully packaged and returned to the Manufacturer, postage prepaid. Any loss or damage during shipment is at the risk of the sender.

C. Conditions of Warranty: The warranty is void if the Pump has been 1) repaired by someone other than the Manufacturer or its authorized agent; 2) altered so that its stability or reliability is affected; 3) misused; or, 4) damaged by negligence or accident. Misuse includes, but is not limited to, use not in compliance with the Operator’s Manual or use with nonapproved accessories. The Pump is a sealed unit, and the fact that the seal has been broken will be considered conclusive evidence that the Pump has been altered or misused. Removal or damage to the Pump’s serial number will invalidate this warranty.

D. Limitations and Exclusions: Repair or replacement of the Pump or any component part thereof is the **EXCLUSIVE** remedy offered by the Manufacturer. The following exclusions and limitations shall apply:

1. No agent, representative, or employee of the Manufacturer has authority to bind the Manufacturer to any representation or warranty, expressed or implied.
2. **THERE IS NO WARRANTY OF MERCHANTABILITY OR FITNESS OR USE OF THE PUMP FOR ANY PARTICULAR PURPOSE.**
3. The Pump can only be used under the supervision of medical personnel whose skill and judgment determine the suitability of the Pump for any particular medical treatment.
4. All recommendations, information, and descriptive literature supplied by the Manufacturer or its agents are believed to be accurate and reliable, but do not constitute warranties.

E. Computer Program License:

1. The Pump is intended to be used in conjunction with a particular Licensed Computer Program supplied by Manufacturer and use of any other program or unauthorized modification of a Licensed Computer Program shall void Manufacturer’s warranty as set forth above.
2. The Original Purchaser and any users authorized by the Original Purchaser are hereby granted a nonexclusive, nontransferable license to use the Licensed Computer Program only in conjunction with the single Pump supplied by Manufacturer. The Licensed Computer Program is supplied only in machine-readable object code form and is based upon Manufacturer’s proprietary confidential information. No rights are granted under this license or otherwise to decompile, produce humanly readable copies of, reverse engineer, modify or create any derivative works based upon the Licensed Computer Program.
3. All other terms and conditions of this Limited Warranty shall apply to the Licensed Computer Program.

The Manufacturer disclaims responsibility for the suitability of the Pump for any particular medical treatment or for any medical complications resulting from the use of the Pump. The Manufacturer shall not be responsible for any incidental damages or consequential damages to property, loss of profits, or loss of use caused by any defect or malfunction of the Pump.

This warranty gives the Original Purchaser specific legal rights, and the Original Purchaser may have other legal rights which may vary from state to state.

Deltec

SIMS Deltec, Inc., St. Paul, MN 55112 U.S.A.

sim SMITHS INDUSTRIES
Medical Systems

© 2000 SIMS Deltec, Inc.
All rights reserved.
Printed in U.S.A.



*Use CADD® pump
accessories carrying
this symbol*

2000-03
40-3660-01H